

1 Measuring single-cell susceptibility 2 to antibiotics within monoclonal 3 bacterial populations

4 Lena Le Quellec^{1,2†}, Andrey Aristov^{1†}, Salomé Gutiérrez Ramos^{1,2},
5 Gabriel Amselem^{1,2}, Julia Bos³, Zeynep Baharoglu³, Didier Mazel³,
6 Charles N. Baroud^{1,2*}

*For correspondence:

charles.baroud@pasteur.fr (CNB)

†These authors contributed
equally to this work

7 ¹Physical Institut Pasteur, Université Paris Cité, Microfluidics and
8 Bioengineering Unit, 75015 Paris, France; ²LadHyX, CNRS, Ecole
9 polytechnique, Institut polytechnique de Paris, 91120, Palaiseau, France;
10 ³Institut Pasteur, Université Paris Cité, CNRS UMR3525, Bacterial
11 Genome Plasticity Unit, F-75015 Paris, France

12

13 **Abstract** Given the emergence of antimicrobial drug resistance, it is critical to
14 understand the heterogeneity of response to an antibiotic within a population of cells.
15 Since the drug can exert a selection pressure that leads to the emergence of resistant
16 phenotypes. To date, neither bulk nor single-cell methods are able to link the
17 heterogeneity of single-cell susceptibility to the population-scale response to antibiotics.
18 Here we present a platform that measures the ability of individual *E. coli* cells to form
19 small colonies at different ciprofloxacin concentrations, by using anchored microfluidic
20 drops and an image and data analysis pipelines. The microfluidic results are
21 benchmarked against classical microbiology measurements of antibiotic susceptibility,
22 showing an agreement between the pooled microfluidic chip and replated bulk
23 measurements. Further, the experimental likelihood of a single cell to form a colony is
24 used to provide a probabilistic antibiotic susceptibility curve. In addition to the
25 probabilistic viewpoint, the microfluidic format enables the characterization of
26 morphological features over time for a large number of individual cells. This pipeline
27 can be used to compare the response of different bacterial strains to antibiotics with
28 different action mechanisms.

29

30 Introduction

31 Antimicrobial resistance is considered by the World Health Organization as one of the
32 biggest threats to public health [25]. Developing new tools and methods to better under-
33 stand bacterial resistance is becoming necessary. When addressing the question of bac-
34 terial response to antibiotics, most microbiology studies report the Minimum Inhibitory
35 Concentration (MIC) at which the cells stop growing, for a given initial inoculum size (usu-
36 ally 10^5 cells) and after a growth time of over 24 hours. However, interpreting these MIC

37 measurements is far from trivial and could indicate many different phenomena taking
38 place in the cultures (high variability, inoculum effect, mechanism of action of the antibiotic)
39 [16]. Indeed, the response of individual cells, which may then lead to colonies, can
40 display large heterogeneity [11, 12]. For this reason the MIC is sometimes complemented
41 with a more precise measurement, the Minimum Bactericidal Concentration (MBC). The
42 process of determining the MBC is heavy and time-consuming and, like the MIC, only
43 gives information about the antibiotic susceptibility on the population level. This has mo-
44 tivated significant effort to measure the bacterial response at a more microscopic level.

45 For instance, a single-cell MIC was estimated by measuring the MIC for different inocu-
46 lum sizes and extrapolating the value to a single cell [5]. Classical laboratory methods,
47 however, are difficult to scale to single-cell manipulation, both in terms of the volumes
48 of interest and also the number of experiments that are required to obtain a significant
49 number of replicates. In contrast, the development of microfabrication methods and mi-
50 crofluidics has allowed measurements to be made on individual cells in controlled envi-
51 ronments [6]. In this area, two platforms which address questions of antibiotic response
52 have emerged. First the so-called mother machine and its variations, where individual
53 cells are trapped in thin channels and observed over a large number of generations [28].
54 These devices rely on the tracking of the initial *mother* cells by time-lapse microscopy,
55 while removing its daughter cells as they push out of the microchannels. By fine analysis
56 of the images under different antibiotic treatments it is possible to learn about relations
57 between mother and daughter cells [9], or to detect the effect of rare mutations on the
58 fitness at the single-cell level [26].

59 In parallel, the field of droplet microfluidics has allowed studies of a different kind. By
60 encapsulating one or a few bacterial cells within water-in-oil droplets, the development of
61 small colonies from individual cells [15], or the signature of their metabolism [10], can be
62 detected with optical readouts. The addition of antibiotics in solution within the droplets
63 can then be used to determine the bacteria's susceptibility. This basic principle has, in
64 recent years, been developed in two main directions. Either to improve the simplicity of
65 use [13, 19] or to improve the precision of the measurements [22, 23, 27]. These droplets
66 approaches have the potential to be transferred to clinical studies, as reviewed in recent
67 papers [18, 30, 14].

68 Although these droplet methods constitute important milestones, they suffer from
69 several drawbacks: First, they require specific and sophisticated equipment including pre-
70 cise flow control systems to ensure droplet size homogeneity, as well as high-speed elec-
71 tronics, lasers, and data acquisition, to perform the measurements on flowing droplets.
72 Second, the latest methods do not allow the droplets to be followed in time or to relate
73 the final state to the initial state of the droplets. Finally, the link between the single-
74 cell measurements and the classical biological measurements has never been explicitly
75 tested. As such, it is difficult to relate the droplet-based measurements with the vast
76 quantity of data obtained in traditional experiments.

77 Here, we present an open-access microfluidic platform that addresses some of these
78 issues. The platform is based on *rails and anchors* that were introduced a few years
79 ago [1]. Those droplets are formed within microfabricated wells and remain stationary
80 for the duration of the experiment, including for the observation of biological processes
81 within them [2, 3]. As such, the platform only requires simple microfabrication, low-
82 precision flow control and allows to complete time-lapse measurements. The microflu-

83 idic setup is augmented with an original and dedicated image acquisition and analysis
84 pipeline that extracts the relevant information from the chips in an automated manner.
85 By providing the image and data analysis as open-source code, the platform will be easy
86 to integrate in most academic laboratories. Moreover, the current study addresses the
87 interpretation of the biological measurements for the first time. By doing so it links the
88 droplet-level approach, used in most droplet-based experiments, with a single-cell anal-
89 ysis. This analysis is used to obtain unique measurements of the single-cell susceptibility
90 to antibiotics.

91 **Results**

92 **Microfluidic platform and initial observations**

93 The microfluidic device used in this study is based on a geometry described previously [3,
94 4]. It consists of a triangular array of 501 individual wells, or anchors, that can each hold a
95 single aqueous droplet (Fig. 1a). The chip format is well suited for imaging on an inverted
96 microscope, either using wide-field illumination or confocal mode, as discussed below.

97 Loading the chip and distributing the bacterial solution into droplets is straightfor-
98 ward and takes about 5 min (see Method for the detailed steps, and Fig. 1 b, c, d). Briefly,
99 the device is first entirely filled with oil (FC40, 3M) containing 0.5% surfactant (FluoSurf,
100 EmulSEO, France). Then, the aqueous suspension of bacteria is flowed through the device.
101 In a last step, the oil is flowed again through the device, which leads to the formation and
102 immobilization of droplets containing bacteria, directly on the anchors. The volume of
103 each droplet is 2 nl and is primarily determined by the volume of the anchor [2]. This load-
104 ing procedure is simple to set up and can be mastered in only a couple of trials. Indeed,
105 the droplet formation step is robust to fluctuations in flow rate. It can be performed using
106 syringe pumps or using hand-held syringes. Also note that the whole loading procedure
107 is performed while the output is connected to a waste tube, and the bacterial suspen-
108 sion is constantly encapsulated in an inert oil layer. This makes the protocol suitable in
109 principle to handling pathogens, since the bacterial solution remains in a closed circuit.

110 *E. coli* W3110 with a fluorescent reporter (RFP) in the ptac site (ptac::RFP) allows us
111 to detect bacterial cells and the growth of the colonies using the red fluorescent protein
112 (RFP) . A sample fluorescence image of the trapping area of the chip, acquired after 24
113 hours of incubation, is shown in Fig. 1e. The bacteria at this stage form bright fluorescent
114 colonies that can readily be imaged using epifluorescence or confocal microscopy. Empty
115 droplets are also present on the device, since the cells are randomly distributed. The
116 number of empty droplets is related to the average number of bacteria per drop, which
117 is in turn related to the initial concentration of the bacterial suspension. Starting from
118 different initial dilutions, therefore, allows us to tune the average number of cells per
119 droplet and the number of positive droplets within the chip in the absence of antibiotics.

120 Before moving on to testing the effects of antibiotics in the microfluidic device, we to
121 benchmark the bacterial fitness in the microfluidic device compared with standard multi-
122 well plate experiment. This is done by following the growth of the fluorescent intensity in
123 the droplets, using time-lapse epifluorescence microscopy, while performing in parallel
124 a standard growth-curve measurement on a fluorescence plate reader from the same
125 batch culture. The growth curves for the two cases are shown in Fig. 1f. The curves from
126 the microfluidic device show a large variability between individual droplets, as a result

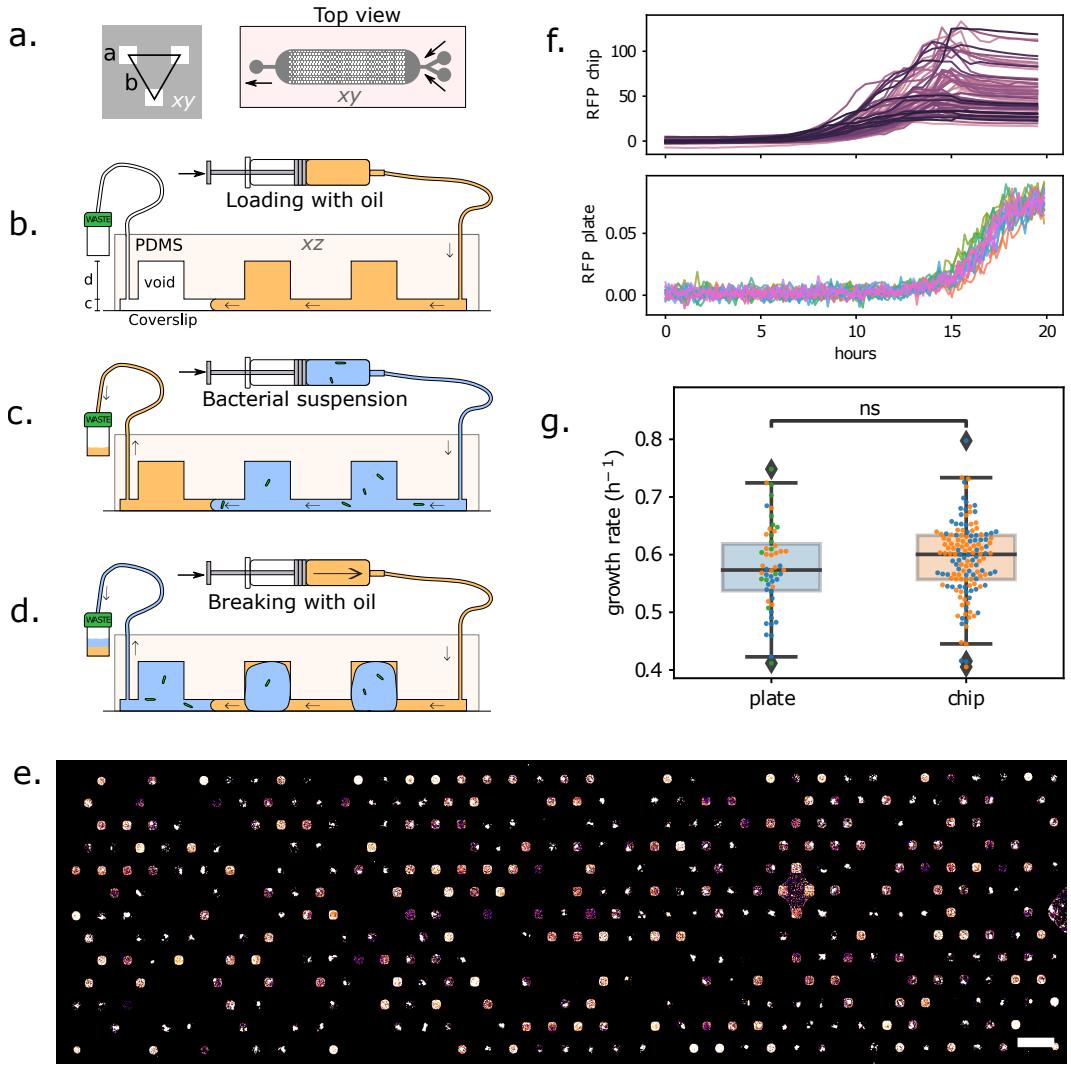


Figure 1. (a) Microfluidic chip design. Left: a unit cell consists of a triangular arrangement of square anchors, each of size $a = 120 \mu\text{m}$ and distance $b = 360 \mu\text{m}$. Right: design of the full chip, which includes a main chamber with 501 anchors, 2 input channels on the right and 1 outlet channel on the left. **(b)** Side-view (not to scale), showing the channel height $c = 30 \mu\text{m}$ and anchor depth $d = 100 \mu\text{m}$. The loading protocol begins by filling the chamber with oil, then **(c)** replacing the oil with bacterial suspension, and **(d)** breaking the bacterial suspension into individual droplets, anchored in their respective wells. **(e)** Z-projection of a confocal stack of the chip after 24 h incubation (scalebar: 500 μm). **(f)** Growth curves in 501 individual droplets on the chip (top), and in each well of a 96-well plate (bottom). **(g)** Measured growth rates for bacteria in the microfluidics chip (2 replicates), and in the 96-well plate (3 replicates). Growth rates were obtained by fitting an exponential function to the growth curves during the first 10 hours of growth. P-value=0.24 obtained with Welch's t-test for independent samples.

127 of distribution of the number of initial cells and of the cell-to-cell variability [7]. In con-
128 trast, the multiwell plate experiments are insensitive to these stochastic elements and
129 grow in a reproducible and regular manner. Fitting the individual growth curves with an
130 exponential function for the first 10 hours of growth shows that the difference in growth
131 rates in the microfluidic device and in the multiwell plates is statistically not significant,
132 see Fig. 1g. Hence, the microfluidic results can be compared to standard microbiology
133 techniques.

134 **Imaging and analysis pipelines**

135 Once the microfluidic device is loaded, the aim of the experiments is to identify which
136 droplets within the array produce a population of cells after 24h and to link the final state
137 with the initial number of cells in each droplet. These measurements are performed
138 by first imaging the chip shortly after the loading and then after overnight incubation.
139 Image analysis of the initial and final time points then yields a table that identifies each
140 droplet in the array. Each droplet is then associated with measured quantities such as
141 the initial number of cells, its final state, as well as the antibiotic concentration for a given
142 experiment (see schematic in Fig. 2).

143 As such, the ability to acquire and analyze large amounts of imaging data is funda-
144 mental to obtain the antibiotic response curves. While the array format lends itself nat-
145 urally to measuring droplet contents at different time points, the requirement to detect
146 single cells at early times imposes high-resolution imaging. This runs into data han-
147 dling limitations associated with the large file sizes and large number of experiments.
148 These different constraints led us to develop automated imaging and analysis pipelines
149 whose implementation was instrumental for obtaining the results below. The imaging
150 steps are described below and the image and data analysis pipelines are provided as
151 open-source packages at the following GitHub repository: <https://github.com/BaroudLab/anchor-droplet-chip>.

152 The aim of the pipeline is to generate a table with one line for each droplet, which
153 includes a unique label, the antibiotic concentration, as well as the initial number of cells
154 and final state for the droplet, as described in Fig. 2.

156 **Initial state.**

157 The initial number of cells per droplet is obtained by imaging the freshly loaded chip first
158 in bright-field, and second by acquiring a confocal z-stack of the device in the RFP chan-
159 nel. The bright-field image is used to detect the positions of the droplets, by adjusting for
160 arbitrary shift and tilt of each acquisition (see Methods). In turn, the confocal stack is re-
161 duced to a single image by using a maximum projection of the fluorescent intensity. The
162 resulting fluorescent image allows us to count the number of individual bacteria within
163 each droplet (Fig. 2c). The algorithm proved sufficiently robust to perform unsupervised
164 automated analysis of the data from the chips.

165 Since the cells are expected to follow a Poisson distribution in the droplets [3], a quick
166 quality control is performed at the end of the first scan, by verifying the distribution of
167 number of cells per droplet, and checking that it indeed follows the expected shape, see
168 Fig. 2i. This calculation also allows us to obtain a value of the Poisson parameter λ and
169 to adjust the cell dilution if necessary in order to work in the desired range of λ .

170 Note that the loading and scanning each take about 10 minutes and the initial image

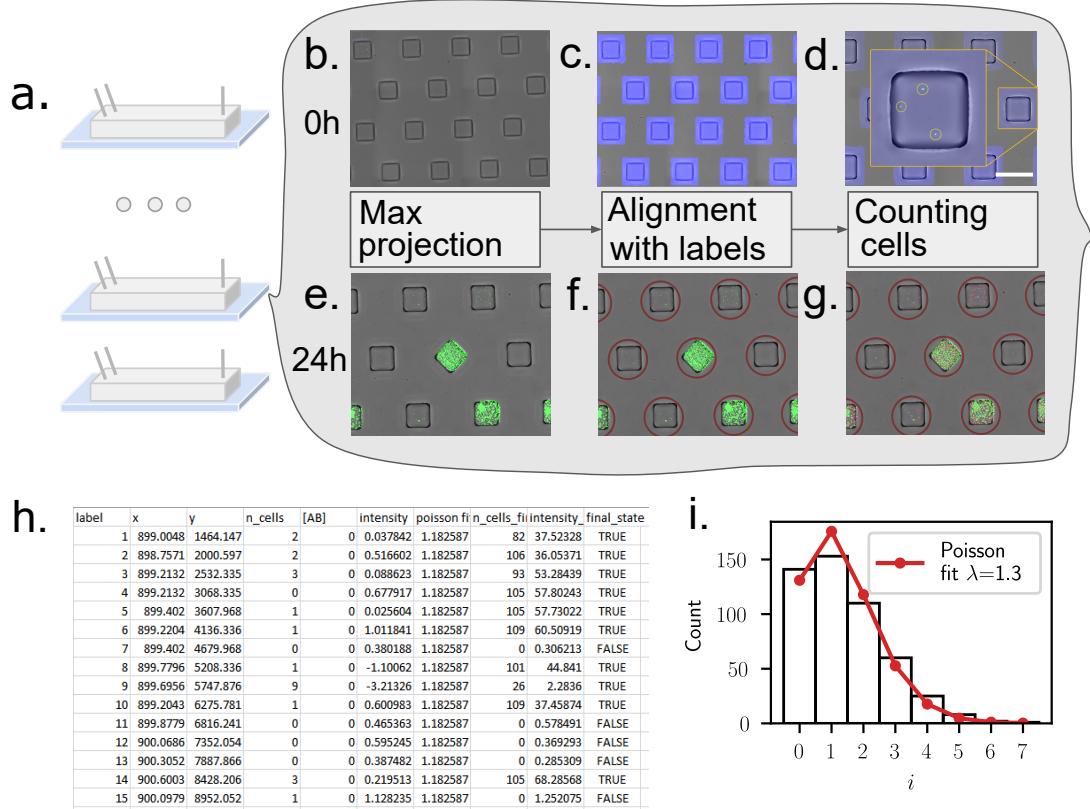


Figure 2. Imaging and image analysis pipeline. **(a)** The experiment begins by loading several chips with bacterial suspensions at different antibiotic concentrations. **(b)** Overlay of the bright-field image of the chip, and of the maximum projection of a fluorescent confocal z-stack. Images are acquired minutes after loading (0 h). **(c)** The bright-field image is used to identify the alignment with respect to the microscope stage and to create a unique mask around the positions of the individual anchors. **(d)** Detecting the fluorescent peaks in the maximum projection enables to count the initial number of cells per droplet. **(e)-(g)** Similar imaging and analysis operations are performed 24 h after the loading, to identify positive and negative droplets. **(h)** The data from the initial and final images are collected in a table that provides a unique label for each droplet, as well as the number of cells at 0 h and at 24 h. Each droplet is assigned a final status of positive or negative, depending on whether the final number of cells is larger than a predefined threshold of 15 cells. **(i)** A quality control step is performed using the single-cell detection at $t = 0$ by comparing the cell number distribution with a Poisson distribution. This leads to an estimate of the Poisson parameter λ for each chip.

171 validation occurs within a few minutes as well. This yields a first measurement of the
172 loading in under 30 minutes for each microfluidic chip.

173 Final state.

174 The contents of each droplet are later measured at the experimental endpoint, typically
175 after an overnight incubation ($t = 18 - 24$ h): each chip is scanned, this time using simple
176 epi-fluorescence to optimize time and disk storage. The final image of each chip is re-
177 aligned with the template acquired at initial times to identify each droplet, a registration
178 step made straightforward by the fact that droplets are anchored at predefined positions.
179 Then, cells are detected within each droplet, as shown in Fig. 2e-g. In the current exper-
180 iments, we focus on the bottom of the microfluidic device where cells are more likely to
181 be detected if the droplet is positive. Different quantities can be obtained from the final
182 image as proxies for the ability of cells to grow within the drop. We count the number of
183 cells in the final image, although mean or total fluorescence intensity can also be used.
184 The main requirement for the measurements is to be sufficiently robust to yield a cutoff
185 between positive and negative droplets, a classification which is also included in the data
186 table. The final result is a csv table that contains the relevant information on the initial
187 and final states of each droplet within each microfluidic device.

188 Note that the protocols described above can be modified for particular situations. For
189 instance time-lapse microscopy can be performed on the chips to obtain time-resolved
190 measurements. Similarly, confocal imaging can be used at later times to obtain a more
191 precise cell count or fluorescent intensity, or to identify the morphology of the cells. Al-
192 though these cases would require small modification in the pipeline, the main bricks of
193 the analysis discussed above can still be used in a modular fashion.

194 **Microfluidic vs. microplate antibiogram**

195 The microfluidics and imaging protocols described above can be combined to obtain an
196 antibiotic susceptibility curve, by loading several chips in parallel, using known concen-
197 trations of antibiotics and bacteria in each chip. Performing these measurements is sim-
198 plified by the standardized microfluidic format and analysis codes, making it possible to
199 run six to twelve chips in parallel, each with a different concentration. Confronting the
200 microfluidic measurements against standard microbiological techniques proves crucial
201 to understand how to interpret the microfluidics data.

202 In each experimental run, one chip is loaded with the same bacterial concentration
203 as the others but without any antibiotic. This control chip allows us to estimate the value
204 of the average number of cells per droplet at initial times, λ , for the given run:

$$\lambda \simeq -\ln(\hat{p}_-), \quad (1)$$

205 where \hat{p}_- is the fraction of empty to total droplets on the test chip. This estimate comes
206 from the assumption that the initial number of cells per droplet follows a Poisson distri-
207 bution [7]. A higher value of λ means that drops contain a larger average number of cells
208 initially.

209 A typical set of images from the experimental endpoint is shown in Fig. 3a. In these
210 images the bright spots correspond to droplets where bacteria grew, while dark spots
211 within the regular matrix correspond to droplets that do not contain a sufficient popula-
212 tion of cells. These dark positions correspond either to droplets that did not contain any

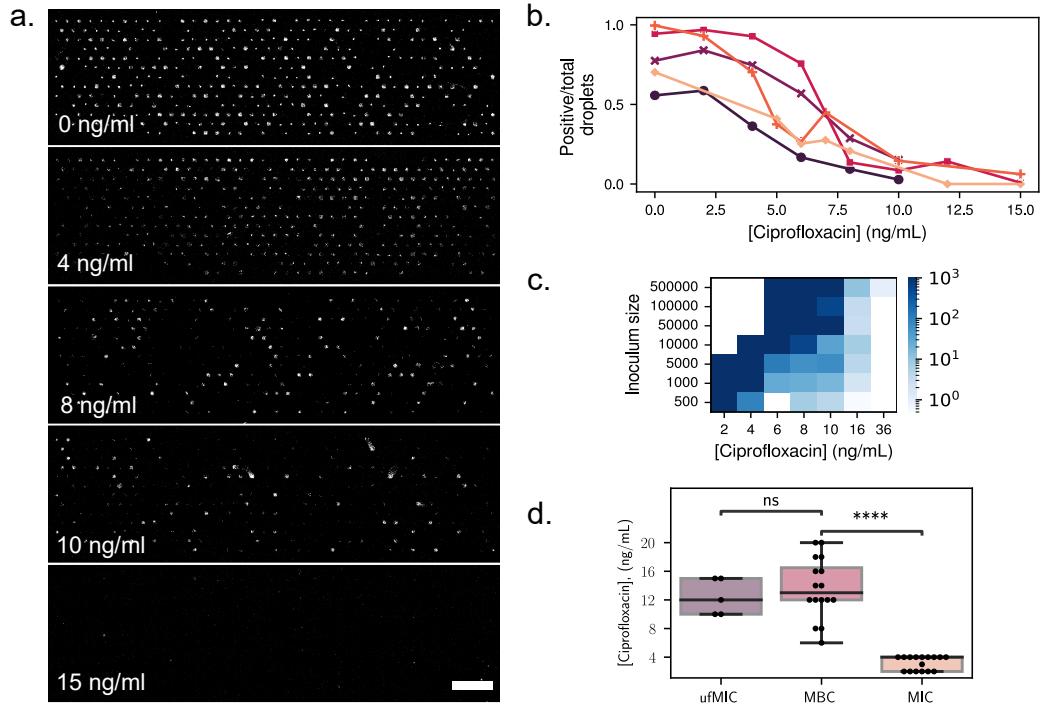


Figure 3. (a) Antibiogram chips with different concentrations of ciprofloxacin, and an initial average number of cells per droplet $\lambda = 1.3$. Bright spots correspond to droplets where bacterial growth occurred. Scale bar: 1 mm. Fraction of positive droplets at the end of the experiment, normalized by the total number of droplets containing at least one bacterium at the beginning of the experiment, for different concentrations of ciprofloxacin. Each color corresponds to a different run, at a different date and with a different value of λ . **(c)** Result of MBC experiments. Bacteria were grown in 96-well plates under different antibiotic concentrations, and starting with different inoculum sizes. The wells were scanned after 24 hours, and the contents of negative wells were replated on antibiotic-free petri dishes for 24 additional hours. The number of colonies on the petri dishes after incubation directly represents the number of surviving bacteria in each well. The color corresponds to the number of colonies on the petri dishes. **(d)** Values of the MBC (petri dishes), MIC (96-well plates) and μ -MIC on the chip, where the total number of cells per chip is used as inoculum size. P-values 6e-8 for MBC vs. MIC and 0.9 for ufMIC vs MBC obtained with Welch's t-test for independent samples.

213 cells initially or to droplets where the cells did not form colonies e.g. due to the antibiotic
214 stress. This antibiogram, allows to determine a measure of the antibiotic susceptibility
215 of the bacteria, which we denote $\mu\text{-MIC}$. The $\mu\text{-MIC}$ corresponds to the lowest antibiotic
216 concentration that will inhibits the growth in 95% of the droplets.

217 As expected, the fraction of positive droplets decreases as the concentration of an-
218 tibiotics is increased. This decrease is quantified in Fig. 3b, where the number of pos-
219 itive droplets is shown to decrease towards zero as the concentration of the antibiotic
220 ciprofloxacin increases, independently of the value of λ .

221 The interpretation of this “digital” measurement and its relation with classical micro-
222 biology measurements is not obvious. To understand its significance, measurements
223 from the microfluidic format were confronted with measurements in a standard mul-
224 tiwell plate, using the same samples. Two classical microbiology measurements were
225 performed on the samples. First, the minimum inhibitory concentration (MIC) was deter-
226 mined with a standard microtitre broth dilution method (see Methods). The MIC corre-
227 sponds to the lowest antibiotic concentration that will inhibits visible growth. Then, the
228 minimum bactericidal concentration (MBC) was obtained by replating the contents of the
229 negative wells on antibiotic-free petri dishes. The number of colonies on the petri dishes
230 after 24 hours of incubation directly represents the number of surviving bacteria in each
231 well. The MBC thus provides a more precise measure of the antibiotic concentration
232 that is lethal to the bacteria, compared to the MIC. We find that the number of colonies
233 growing from negative wells is very large below a critical value of the ciprofloxacin con-
234 centration of 10 ng/mL, after which it drops dramatically to below ≈ 100 colonies, and
235 eventually asymptotes to zero with increasing antibiotic concentration, see Fig. 3c.

236 A comparison of the measurements obtained from the three techniques ($\mu\text{-MIC}$, MIC,
237 and MBC) is shown in Fig. 3d, as a function of inoculum size. The inoculum size used for
238 the $\mu\text{-MIC}$ corresponds to the total number of cells per chip. The classical MIC measure-
239 ment (at $t = 24$ h) is shown to be the least sensitive of the three measurements, since it
240 finds a critical value of the concentration that is well below the value that is necessary
241 to kill all of the cells. In contrast, the values of the MBC and of the $\mu\text{-MIC}$ are in the
242 same range. They both show similar trends with the inoculum size, namely a slow but
243 detectable increase with the initial number of bacterial cells.

244 This close correspondence between the MBC and the $\mu\text{-MIC}$, obtained by pooling
245 together the total number of cells in the chip, indicates that the results in the microfluidic
246 chip can be treated as a population-level measurement: all the bacteria from a single chip
247 form a small population, whose ability to survive to a given concentration of antibiotics
248 depends on its initial size. This result indicates that cells are behaving in an independent
249 manner.

250 **Computing single-cell antibiotic susceptibility**

251 Beyond population level measurements, the objective is to provide insights about the an-
252 tibiotic susceptibility of individual cells within a monoclonal population. This is achieved
253 by taking a probabilistic viewpoint on the ability for a single cell to produce a colony at a
254 given antibiotic concentration. Experimentally, we count the number of bacteria in each
255 droplet at the beginning and at the end of an experiment for six antibiotic concentrations,
256 see Fig. 4a. At the end of an experiment, the image analysis algorithm counts the number
257 of bacteria at the bottom of the droplets. While this number does not reflect the exact

258 total number of cells in the droplet at late times, it is an acceptable proxy to differentiate
 259 positive from negative droplets .

260 A threshold value to distinguish positive from negative droplets is chosen at $n_{\text{final}} =$
 261 15 cells to separate best the two populations (colony or no colony). The number of pos-
 262 itive and negative droplets for each condition and each initial number of cells is then
 263 determined. As a result, the probability of a droplet to contain a colony at the end-point
 264 can be plotted as a function of its initial number of bacteria i , and of the antibiotic con-
 265 centration C_{AB} . We call this probability $p(i, C_{\text{AB}})$: it represents the probability to produce
 266 a colony starting from i cells, under a concentration of antibiotics C_{AB} . The evolution of
 267 p is shown as a heat-map in Fig. 4b. We observe that $p(i, C_{\text{AB}})$ decreases as the antibiotic
 268 concentration increases, but that it increases with the initial number of cells in a droplet;
 269 when more cells are in a droplet initially, more antibiotics are needed to prevent the
 270 growth of a colony after an overnight incubation.

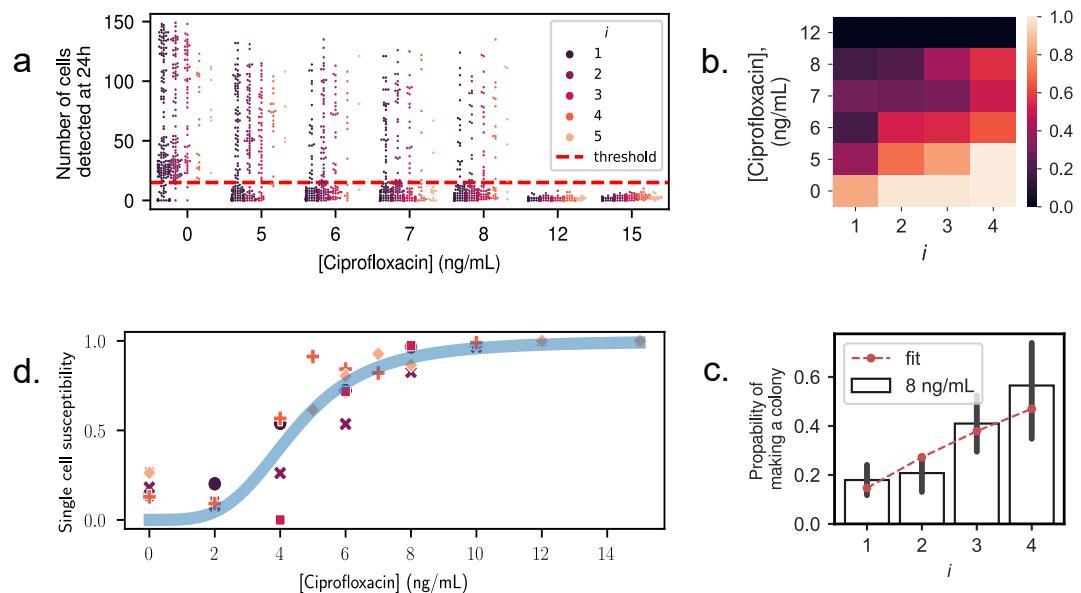


Figure 4. Single-cell antibiotic susceptibility. **(a)** Final number of cells, counted at the bottom of each droplet at $t = 24 \text{ h}$, as a function of antibiotic concentration. Colors indicate the initial number of cells i in the droplet at $t = 0$. The horizontal dashed line is the threshold, fixed at 15 cells, chosen to define the final droplet state as positive or negative. **(b)** Survival probability, computed using Eq. (3), as a function of the initial cell number i and antibiotic concentration. **(c)** The probability to produce a colony as a function of initial number of cells, for $C_{\text{AB}} = 8 \text{ ng/mL}$. Bars indicate experimental measurements from counting positive cells. Dashed line shows fit according to Eq. (2), assuming independent outcomes for each cell and fitting for q . For additional fits, see Supp. Fig. S1 **(d)** The single-cell antibiotic susceptibility is plotted for all antibiotic concentrations and all experimental replicates (points). The data is well-fitted with a two-parameter Hill function (line): $h(C_{\text{AB}}) = C_{\text{AB}}^n / (K + C_{\text{AB}}^n)$, with best fit values $n = 3.9$ and $K = 4.4$.

271 Counting the number of bacteria at initial times, and the fraction of positive droplets
 272 at the end of the experiment, enables to infer the susceptibility of a single cell to a con-

273 centration of antibiotic C_{AB} . This single-cell susceptibility, which we denote $q(C_{AB}) =$
274 $1 - p(1, C_{AB})$, is defined as the probability for a single cell to die (equivalently not form
275 a colony) at concentration C_{AB} . If additionally all bacteria are assumed to behave inde-
276 pendently, the probability for i cells to die is $q(C_{AB})^i$. The probability for i cells to form a
277 colony is therefore the probability for at least one of them to form a colony, and we then
278 have:

$$p(i, C_{AB}) = 1 - q(C_{AB})^i. \quad (2)$$

279 For each concentration of antibiotics, the probability $p(i, C_{AB})$ was estimated by count-
280 ing the number \mathcal{N}_i of droplets containing exactly i cells at the beginning of the experi-
281 ment. Among these \mathcal{N}_i droplets, a number $N^+(i, C_{AB})$ droplets were positive at the end
282 of the experiment. We then have:

$$p(i, C_{AB}) = \frac{N^+(i, C_{AB})}{\mathcal{N}_i}. \quad (3)$$

283 The probability $p(i, C_{AB})$ was fitted to the functional form of Eq. (2) with $q(C_{AB})$ as a
284 single fit parameter, as shown in Fig. 4c (see SI Fig. S1 for all data). The good agreement
285 between the data and the theory confirms that the bacteria may indeed be considered
286 as independent of each other (see in Fig. 4c), at least for the low number of cells present
287 initially at the beginning of the experiments. Then if we write $q^*(C_{AB})$ the best fit value
288 of $q(C_{AB})$, this value provides the best estimate of the single-cell susceptibility to drug
289 concentration C_{AB} , using all experimental data at hand and assuming that all cells are
290 independent.

291 The single-cell susceptibility $q^*(C_{AB})$ is expected to take a sigmoidal shape, with a
292 value near 0 in the absence of drugs (all bacteria form colonies), and increases non-
293 linearly with the drug concentration until reaching a plateau at $q^*(C_{AB}) = 1$. This is con-
294 firmed by the experimental measurements, as shown in Fig. 4d. These data are arbitrarily
295 fitted to a Hill function: $h(C_{AB}) = C_{AB}^n / (K + C_{AB}^n)$, with K and n being two fit parameters,
296 providing a good match between experiments and the fitted function.

297 **Identifying morphology changes under antibiotic stress**

298 This microfluidic device and image analysis pipeline is a very powerful tool to obtain quan-
299 titative information at the single-cell level as seen in Fig. 4. But more than quantitative
300 information, the anchored droplet format provides a unique ability to access qualitative
301 data and to follow the evolution of the bacterial colonies within each droplet over time.
302 The tracking of the droplet contents can be performed by time-lapse microscopy on the
303 chips. Since the droplet position is invariant throughout the experiment, identifying the
304 progeny of an individual cell can be achieved. Examples of a sample droplet contents can
305 be seen in Fig. 5 and the accompanying movies, first in the absence of antibiotics (Fig. 5a)
306 or under a sub-MIC concentration of ciprofloxacin (Fig. 5b).

307 In the absence of antibiotics, almost all droplets display bacteria in their planktonic
308 state, swimming in the droplets and showing the typical size and shape for *E. coli* in cul-
309 ture. A few hours into the experiments and as the populations begin to grow, cells in
310 some droplets start to adhere to each other, eventually forming clumps. The presence
311 of these clumps could be attributed to the presence of adhesion proteins like fimbrial
312 adhesins that may then contribute to biofilm formation of *E. coli* [8, 21].

313 The morphological change of bacteria in the presence of antibiotics often begins with
314 the elongation of the cells into long filaments: this corresponds to 83% of cases in the

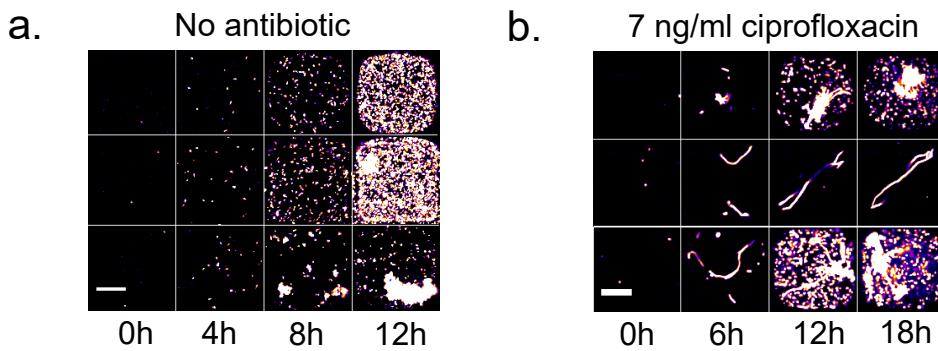


Figure 5. Example of bacterial growth in three independent droplets growth **(a)** without antibiotic, and **(b)** with sub-MIC concentrations of ciprofloxacin (7 ng/mL). Scale bar: 50 μ m. Even at sub-MIC concentrations, the presence of ciprofloxacin leads to a filamentous bacterial morphology.

315 experiments at sub-MIC antibiotic concentration (7 ng/mL). The filamentation is due to
316 the SOS response triggered by the presence of ciprofloxacin; cell-division stops but the
317 cell metabolism continues, leading to cell volume growth. The elongated cells can then
318 begin to produce offspring after several hours (50% of all cases) or can arrest their growth
319 and stay in the filamentous form (33% of all cases). This is in agreement with observations
320 on agar plates [11].

321 In some cases, no elongation is found. These droplets correspond either to cells that
322 were in a dormant state (10% of all cases is expected) [17] or to cells that suffered too
323 much damage and died due to the antibiotics (7% of all cases) as no fluorescence can
324 be detected. As a result of these dynamics, nearly all of the droplets that form colonies
325 contain cells having the filamentous form as well. Nevertheless, the ability to image the
326 contents of the droplets provides a very precise indication of the state of the cells within
327 them. This in turn is informative about the ability of the cells to overcome the antibiotic
328 stress.

329 **Discussion**

330 As the emergence of antibiotic resistance is accelerating, it is crucial to understand the
331 variability of antibiotic response on the single-cell level. This has motivated work using
332 dilution methods to determine the MIC on petri dishes [12] or in liquid media [5], or us-
333 ing precision microscopy on agar [11]. In parallel, microfluidic methods have been used
334 to provide better controlled conditions and statistics over a large number of individual
335 cells [6, 28]. In recent years a flurry of droplet-based approaches has provided informa-
336 tion showing the heteroresistance of a bacterial population [23], digital antibiotic sus-
337 ceptibility [27, 29], or even providing pathogen identification [14]. These droplet-based
338 methods have shown that the encapsulation within droplets can be used to explore the
339 progeny of individual cells as they respond to antibiotic stress. By relying on snapshots of
340 moving droplets, these methods cannot relate the initial and final states of each droplet,
341 nor can they identify the biological mechanisms that allow cells to overcome the antibi-
342 otic stress at sub-MIC concentrations.

343 In this context the device and analysis pipeline presented here combine the advan-
344 tages of microscopy with those of droplet-based methods. Indeed the ability to iden-
345 tify the initial state of each droplet allows us to work at much higher cell numbers per

346 droplet, which translates to similar statistics as previous papers [27] while using a much
347 lower number of droplets in total. Moreover the ability to provide time-resolved measure-
348 ments on each droplet provides unique qualitative information about the adaptation of
349 the cells, similarly to other microscopy-based methods [11]. Finally, the streamlined exper-
350 imental and analysis pipeline allows us to load and image the chip in under 30 minutes,
351 followed by an overnight incubation and a second scan requiring only a few minutes. As
352 a result the complete campaign for obtaining an antibiogram can be performed robustly
353 in a few hours. In contrast, the classical (petri-dish) method requires an initial overnight
354 incubation in a 96 well plate, followed by a second overnight incubation on 50 to 80 petri
355 dishes and manual counting of the colonies thereafter.

356 Beyond the performance aspects, it is important to benchmark the microfluidic mea-
357 surements against standard microbiology protocols. The comparison of MIC, MBC, and
358 μ f-MIC shows that the results in the microfluidic chip can be treated as a population-level
359 measurement, since the μ f-MIC matches the MBC when accounting for the starting inocu-
360 lum size. In addition to this, the detection of individual cells and the ability to perform a
361 large number of single-cell assays in parallel allow us to develop a probabilistic treatment
362 of the outcome within each droplet forming a colony after 24 hours. The probability for
363 an individual cell to produce a colony at a given antibiotic concentration thus describes
364 the heterogeneity of responses in the population.

365 This platform can now be used to address the single-cell response to antibiotics while
366 screening different bacteria and molecules having different mechanisms of action. The
367 expectation is that this screening will translate into both quantitative (shape of the sin-
368 gle cell susceptibility curve) and qualitative (shape of the cells) differences among the
369 conditions. The ability to encapsulate tens or hundreds of cells within the droplets, in
370 a controlled manner, will then allow the exploration of collective behaviors and non-
371 monotonic time-evolution of the response to antibiotics [24]. More complex experiments
372 can also be envisaged, e.g. by recovering the contents of individual drops and perform-
373 ing -omics measurements on them or by varying the antibiotic concentration in time, as
374 described previously [4]. Taken together, the different operations that can be combined
375 into this platform constitute a major step forward in the study of antibiotic response both
376 for scientific questions and for medical applications.

377 Methods

378 Microfluidics and microfabrication

379 Microfabrication and chip design

380 To produce microfluidic chips for the experiments, a custom mold was made using 2-
381 layer-SU-8 photoresist lithography. The bottom layer contains the channels with 2 inputs
382 and 1 output. The upper layer contains inverted microwells of squares shapes 120x120
383 μ m and space 240 μ m apart. As shown in Fig. 1 (a), the wells are organized in 13 rows of
384 39 and 38 wells respectively for odds and even rows. The channel height is 30 μ m and
385 the well height is 130 μ m.

386 Next, PDMS and its curing agent (PDMS SYLGARD 184, Dow Corning) are mixed at a
387 1:10 ratio and poured into the mold. The mold is placed in a vacuum chamber for 30
388 minutes to eliminate air bubbles and then cured for 3 hours at 70 °C. Once the PDMS
389 is cured, the chip is cut off from the mold and plasma bonded (CUTE Plasma, Femto

³⁹⁰ Science) to the coverslip.

³⁹¹ **Hydrophobic treatment**

³⁹² Prior to loading, the chips are surface treated with hydrophobic solution (NOVEC 1720
³⁹³ surface modifier/electronic grade coating 3M). To do so, two surface treatments were
³⁹⁴ done after the plasma bonding by filling the chip with the hydrophobic solution and cur-
³⁹⁵ ing it for 10 minutes at 110°C. A third surface treatment is done prior to loading.

³⁹⁶ **Chip loading**

³⁹⁷ As described in Fig. 1, using a syringe pump (NEMESYS), the chip is first filled through
³⁹⁸ the first input with a continuous oil phase (3M Fluorinert FC40 with non-ionic surfactant
³⁹⁹ RAN fluoSurf final concentration 1 %) while purging the air bubbles. Then, through the
⁴⁰⁰ second input, the continuous oil phase is replaced by the bacterial suspension. Finally,
⁴⁰¹ the continuous oil phase is injected again at a very low flow rate, breaking the droplets
⁴⁰² apart and leaving them locked in the wells.

⁴⁰³ **Cell culture and preparation**

⁴⁰⁴ **Strain**

⁴⁰⁵ The experiments were performed using the *E. coli* W3110 strain JEK1037 [20] labeled with
⁴⁰⁶ red fluorescent protein (lacYZ:RFP).

⁴⁰⁷ **Antibiotic Solution**

⁴⁰⁸ Ciprofloxacin (Sigma-Aldrich) was solubilized in 0.1 N HCl (Sigma-Aldrich) at 25 mg/mL.
⁴⁰⁹ The stock was then diluted with MiliQ water to 1 μ g/mL. The final concentration of ciprofloxacin
⁴¹⁰ used was between 0 and 32 ng/mL.

⁴¹¹ **Cell culture**

⁴¹² From the -80°C stock, the cells were streaked on LB agar plate and incubated overnight
⁴¹³ at 37°C. The next day one isolated colony is inoculated in supplemented minimal media
⁴¹⁴ (MOPS with glucose final concentration 0.4%) and IPTG is added at 0.05 mM to induce
⁴¹⁵ the expression of the RFP. The bacterial suspension is incubated overnight at 37°C with
⁴¹⁶ shaking.

⁴¹⁷ **Cell dilution**

⁴¹⁸ In order to get one to five cells per droplet, the optical density of the solution, measured
⁴¹⁹ at 600nm, was calibrated. This was achieved as follows: the calibration was known by
⁴²⁰ using digital counting : the chip was loaded with the diluted bacterial suspension without
⁴²¹ antibiotics, incubated at 37°C overnight, and then imaged. The empty wells were counted,
⁴²² and assuming a well can only be empty if no cells is loaded, the initial loading parameter
⁴²³ λ was computed. λ is the Poisson parameter which corresponds to the mean number
⁴²⁴ of cells per droplet and can be directly obtained by $-\ln(N_{(-)}/N_{total})$. Where $N_{(-)}$ is the
⁴²⁵ number of negative droplets and N_{total} is the total number of droplets. λ is monitored by
⁴²⁶ the concentration of the bacterial suspension and directly linked to the optical density.

⁴²⁷ **Growth characterization and antibiotic susceptibility**

428 Growth curves

429 For growth characterization cells were loaded at different dilutions (500 to 500,000 cells
430 per well) in a 96-well plate. The plate was then placed in the plate reader (Thermo Sci-
431 entific Varioskan LUX) for 24 hours at 37°C with shaking. The optical density at 600 nm
432 (OD) and the RFP fluorescence signal (excitation 488 nm and emission 520 nm) were mea-
433 sured every 10 minutes.

434

435 In parallel, cells were loaded to the chip with an average of one cell per droplet. This
436 corresponds to one cell per droplet on average. The chip was then placed under the
437 microscope and the RFP signal was measured every 30 minutes.

438 MIC and MBC

439 The minimum inhibitory concentration (MIC) and minimum bactericidal concentration
440 (MBC) were obtained to characterize the antibiotic susceptibility at the population level.

441

442 Cells are loaded in a 96 well plate at different dilutions (500 to 500,000 cells per well)
443 and with different ciprofloxacin concentration ranging from 2 to 36 ng/mL. The plate is
444 then incubated for 24 hours at 37°C with shaking.

445

446 The MIC is determined as the antibiotic concentration of the first negative well, i.e.
447 the well at which the OD is the same as the OD of an empty well.

448 Then, the contents of the negative wells are plated on LB agar plates and incubated
449 for 24 hours at 37°C. The number of colonies from each of these plates is counted. The
450 MBC is determined as the concentration where the number of colonies decrease sharply
451 from more than a hundred cells to less than a dozen cells.

452 Single-cell susceptibility

453 To characterize the single-cell susceptibility to antibiotic, at least 10 microfluidic chips are
454 fabricated and loaded per experiment : a control chip without antibiotic, and nine more
455 with serial concentrations of ciprofloxacin (from 2 to 36 ng/mL). The bacterial suspension
456 is prepared with the antibiotic and immediately loaded into the chip. The chip is imaged,
457 using fluorescence microscopy, right after in order to determine the exact number of
458 cells in each well.

459 Then, the chip is immersed in a container filled with Milli Q water to prevent evapo-
460 ration and incubated overnight at 37°C. After incubation, a scan of each chip, measuring
461 the RFP signal is performed, using fluorescence microscopy.

462

463 Microscopy and image acquisition

464 Microscopy images are acquired using spinning disk confocal microscope (Nikon Ti2 +
465 Yokogawa) with a 20x 0.7 NA air objective lens (Nikon Inc.) and with 2x2 pixels binning
466 (set directly in camera properties (Hammamatsu Orca 4)). Images of the complete chip
467 are obtained by stitching individual images with a 5% overlap. The imaging rate is opti-
468 mized by acquiring first a bright-field image of the complete chip. The RFP signal is then
469 obtained either in confocal mode, using 3D stack.

470 For the 3D stack, using triggered NIDAQ Piezo Z, planes are acquired with a step of
471 1 μm , for a total penetration of 120 μm .

472 The total area of the device is about 1.4 by 0.4 mm, which translates to 40 kpix long
473 dataset using 350 nm pixel size. However, some chips could be tilted due to manual
474 bonding, which effectively increases the necessary scanning area, resulting in much big-
475 ger images.

476 **Image analysis**

477 **Image registration**

478 First the 3D fluorescence stack is converted to 2D using maximum projection (see Fig. S2
479 b,e). Both channels, 2D bright-field and 2D fluorescence images, are merged together
480 and saved as a tif stack. Then a well-labelled template image and a well-labelled mask
481 are made and aligned to the experimental images (see Fig. S2 c,f).

482 Note that the protocols described above can be modified for particular situations. For
483 instance time-lapse microscopy can be performed on the chips, in order to obtain time-
484 resolved measurements. Similarly, confocal imaging can be used at later times in order
485 to obtain a more precise cell count or fluorescent intensity, or to identify the morphology
486 of the cells in particular cases. Although these cases would require small modification
487 in the pipeline, the main bricks of the analysis discussed above can still be used in a
488 modular fashion, without major changes in the general approach.

489 **Cell counting**

490 After image registration, every droplet is associated with the labeled area defined by the
491 mask. Inside this mask, peak detection is performed to detect single fluorescent cells.
492 To avoid false detection, due to noise, a preprocessing is performed as follows: First, a
493 Gaussian filter, and subsequent peak detection using Scipy function peak_local_max with
494 an absolute threshold of two. The number of peak per label is then recorded into a table
495 for further processing.

496 **Acknowledgements**

497 This project was partially funded by ANR grant UniBAC (ANR-17-CE13-0010). The authors
498 would like to thank the support of the Microfluidics and Biomaterials platform at Institut
499 Pasteur. We also thank Erik Maikranz for useful discussions.

500 **Supplementary information**

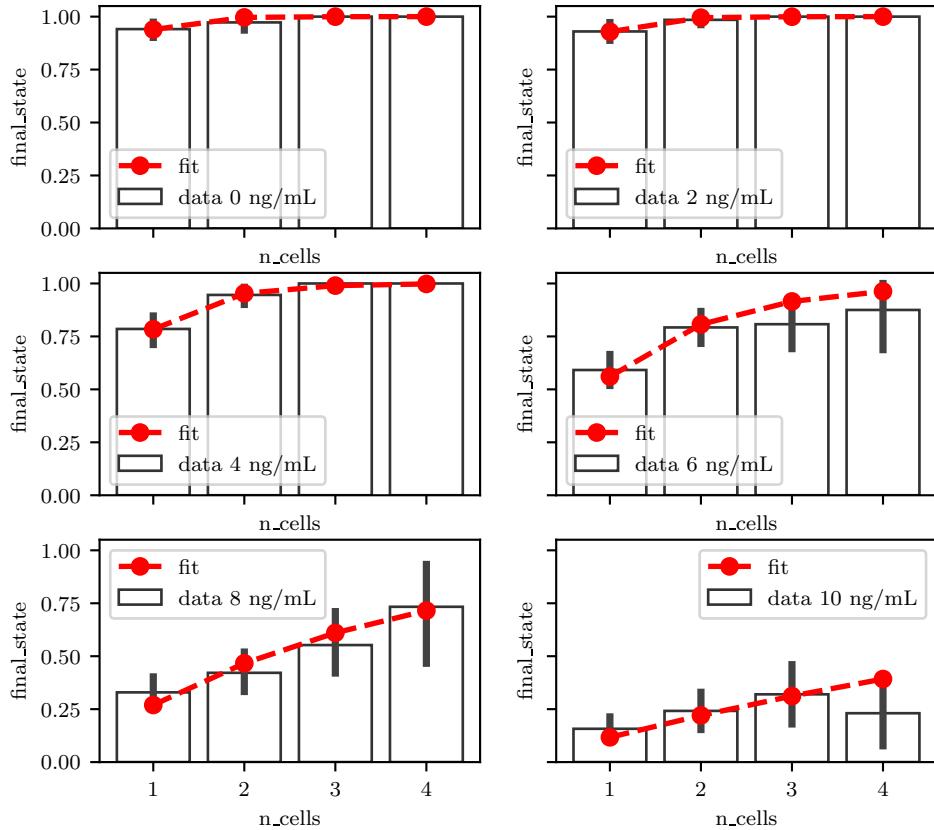


Figure S1. Fitting susceptibility to susceptibility for different concentrations of ciprofloxacin.

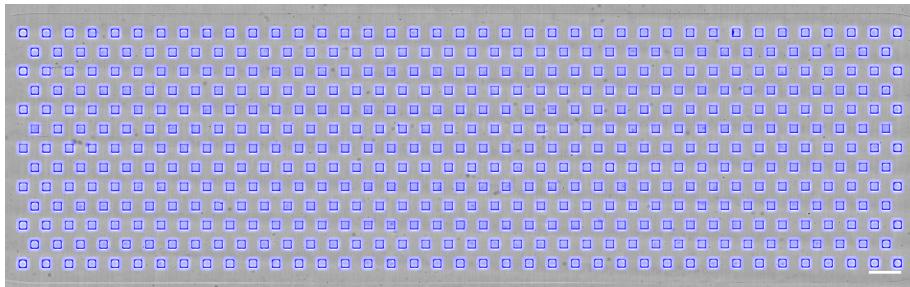


Figure S2. Template (grayscale) + mask (blue) used for alignment and segmenting the droplets. Scalebar 500 μm

501 References

502 [1] **Abbyad P**, Dangla R, Alexandrou A, Baroud CN. Rails and anchors: guiding and trapping
503 droplet microreactors in two dimensions. *Lab on a Chip*. 2011; 11(5):813–821.

504 [2] **Amselem G**, Brun P, Gallaire F, Baroud CN. Breaking anchored droplets in a microfluidic
505 Hele-Shaw cell. *Physical Review Applied*. 2015; 3(5):054006.

506 [3] **Amselem G**, Guermonprez C, Drogue B, Michelin S, Baroud CN. Universal microfluidic plat-
507 form for bioassays in anchored droplets. *Lab Chip*. 2016; 16(21):4200–4211. <http://xlink.rsc.org/?DOI=C6LC00968A>, doi: 10.1039/C6LC00968A, publisher: Royal Society of Chemistry.

508 [4] **Amselem G**, Sart S, Baroud CN. Universal anchored-droplet device for cellular bioassays. In: *Methods in Cell Biology*, vol. 148 Elsevier; 2018.p. 177–199.

509 [5] **Artemova T**, Gerardin Y, Dudley C, Vega NM, Gore J. Isolated cell behavior drives the evolution
510 of antibiotic resistance. *Molecular Systems Biology*. 2015 Jul; 11(7):822. <https://www.embopress.org/doi/full/10.15252/msb.20145888>, doi: 10.15252/msb.20145888, publisher: John Wiley &
511 Sons, Ltd.

512 [6] **Balaban NQ**, Merrin J, Chait R, Kowalik L, Leibler S. Bacterial Persistence as a Phenotypic
513 Switch. *Science*. 2004 Sep; 305(5690):1622–1625. doi: 10.1126/science.1099390.

514 [7] **Barzien A**, Suryateja Jammalamadaka M, Amselem G, Baroud CN. Growing from a few cells:
515 combined effects of initial stochasticity and cell-to-cell variability. *Journal of the Royal Society
516 Interface*. 2019; 16(153):20180935.

517 [8] **Beloin C**, Michaelis K, Lindner K, Landini P, Hacker J, Ghigo JM, Dobrindt U. The transcriptional
518 antiterminator RfaH represses biofilm formation in *Escherichia coli*. *Journal of bacteriology*.
519 2006; 188(4):1316–1331.

520 [9] **Bergmiller T**, Andersson AMC, Tomasek K, Balleza E, Kiviet DJ, Hauschild R, Tkačík G, Guet CC.
521 Biased partitioning of the multidrug efflux pump AcrAB-TolC underlies long-lived phenotypic
522 heterogeneity. *Science*. 2017; 356(6335):311–315. doi: 10.1126/science.aaf4762, ISBN: 1095-
523 9203 (Electronic) 0036-8075 (Linking).

524 [10] **Boedicker JQ**, Li L, Kline TR, Ismagilov RF. Detecting bacteria and determining their suscepti-
525 bility to antibiotics by stochastic confinement in nanoliter droplets using plug-based microflu-
526 idics. *Lab on a Chip*. 2008; 8(8):1265–1272.

527 [11] **Bos J**, Zhang Q, Vyawahare S, Rogers E, Rosenberg SM, Austin RH. Emergence of antibiotic
528 resistance from multinucleated bacterial filaments. *Proceedings of the National Academy of
529 Sciences*. 2015; 112(1):178–183. <http://www.pnas.org/lookup/doi/10.1073/pnas.1420702111>, doi:
530 10.1073/pnas.1420702111, ISBN: 0027-8424 (Print).

531 [12] **Coates J**, Park BR, Le D, Şimşek E, Chaudhry W, Kim M. Antibiotic-induced population fluctu-
532 ations and stochastic clearance of bacteria. *Elife*. 2018; 7:e32976.

533 [13] **Derzsi L**, Kaminski TS, Garstecki P. Antibiotograms in five pipetting steps: precise dilution as-
534 says in sub-microliter volumes with a conventional pipette. *Lab Chip*. 2016; 16(5):893–901.
535 <http://xlink.rsc.org/?DOI=C5LC01151E>, doi: 10.1039/C5LC01151E, publisher: Royal Society of
536 Chemistry ISBN: 1473-0197.

537 [14] **Hsieh K**, Mach KE, Zhang P, Liao JC, Wang TH. Combating Antimicrobial Resistance
538 via Single-Cell Diagnostic Technologies Powered by Droplet Microfluidics. *Acc Chem
539 Res*. 2022 Jan; 55(2):123–133. <https://pubs.acs.org/doi/10.1021/acs.accounts.1c00462>, doi:
540 10.1021/acs.accounts.1c00462.

544 [15] **Huebner A**, Srisa-Art M, Holt D, Abell C, Hollfelder F, Demello A, Edel J. Quantitative detection
545 of protein expression in single cells using droplet microfluidics. *Chemical communications*.
546 2007; (12):1218–1220.

547 [16] **Jepson AK**, Schwarz-Linek J, Ryan L, Ryadnov MG, Poon WC. What is the ‘minimum inhibitory
548 concentration’(mic) of pexiganan acting on *escherichia coli*?—a cautionary case study. In: *Bio-
549 physics of infection* Springer; 2016.p. 33–48.

550 [17] **Jøers A**, Kaldalu N, Tenson T. The Frequency of Persisters in < i > Escherichia coli < /i > Reflects
551 the Kinetics of Awakening from Dormancy. *Journal of Bacteriology*. 2010; 192(13):3379–3384.
552 <https://journals.asm.org/doi/abs/10.1128/JB.00056-10>, doi: 10.1128/JB.00056-10.

553 [18] **Kaminski TS**, Scheler O, Garstecki P. Droplet microfluidics for microbiology: techniques,
554 applications and challenges. *Lab Chip*. 2016; 16:2168–2187. <http://pubs.rsc.org/en/Content/ArticleLanding/2016/LC/C6LC00367B>, doi: 10.1039/C6LC00367B, publisher: Royal Society of
555 Chemistry ISBN: 1473-0197.

557 [19] **Kao YT**, S Kaminski T, Postek W, Guzowski J, Makuch K, Ruszczak A, Stetten Fv, Zengerle R,
558 Garstecki P. Gravity-driven microfluidic assay for digital enumeration of bacteria and for an-
559 tibiotic susceptibility testing. *Lab on a Chip*. 2020; 20(1):54–63. <https://pubs.rsc.org/en/content/articlelanding/2020/lc/c9lc00684b>, doi: 10.1039/C9LC00684B, publisher: Royal Society of Chem-
560 istry.

562 [20] **Keymer JE** **LGLDAR** **Galajda P** . . ; .

563 [21] **Klemm P**. Fimbrial Adhesins of *Escherichia coli*. *Reviews of Infectious Diseases*. 1985 05;
564 7(3):321–340. <https://doi.org/10.1093/clinids/7.3.321>, doi: 10.1093/clinids/7.3.321.

565 [22] **Liu X**, Painter RE, Enesa K, Holmes D, Whyte G, Garlisi CG, Monsma FJ, Rehak M, Craig FF, Smith
566 CA. High-throughput screening of antibiotic-resistant bacteria in picodroplets. *Lab Chip*. 2016;
567 16:1636–1643. <http://dx.doi.org/10.1039/C6LC00180G>, doi: 10.1039/C6LC00180G, publisher:
568 Royal Society of Chemistry ISBN: 8620871129.

569 [23] **Lyu F**, Pan M, Patil S, Wang JH, Matin AC, Andrews JR, Tang SKY. Phenotyping antibiotic
570 resistance with single-cell resolution for the detection of heteroresistance. *Sensors and
571 Actuators B: Chemical*. 2018 Oct; 270:396–404. <https://linkinghub.elsevier.com/retrieve/pii/S0925400518309493>, doi: 10.1016/j.snb.2018.05.047.

573 [24] **Meredith HR**, Andreani V, Ma HR, Lopatkin AJ, Lee AJ, Anderson DJ, Batt G, You L. Applying
574 ecological resistance and resilience to dissect bacterial antibiotic responses. *Science Advances*. 2018;
575 4(12):eaau1873. <https://www.science.org/doi/abs/10.1126/sciadv.aau1873>, doi:
576 10.1126/sciadv.aau1873.

577 [25] **O’Neill J**. Antimicrobial resistance. Tackling a crisis for the health and wealth of nations. 2014;
578 .

579 [26] **Robert L**, Ollion J, Robert J, Song X, Matic I, Elez M. Mutation dynamics and fitness effects
580 followed in single cells. *Science*. 2018; 359(6381):1283–1286.

581 [27] **Scheler O**, Makuch K, Debski PR, Horka M, Ruszczak A, Pacocha N, Sozański K, Smolander OP,
582 Postek W, Garstecki P. Droplet-based digital antibiotic susceptibility screen reveals single-cell
583 clonal heteroresistance in an isogenic bacterial population. *Sci Rep*. 2020 Feb; 10(1):3282.
584 <https://www.nature.com/articles/s41598-020-60381-z>, doi: 10.1038/s41598-020-60381-z, num-
585 ber: 1 Publisher: Nature Publishing Group.

586 [28] **Wang P**, Robert L, Pelletier J, Dang WL, Taddei F, Wright A, Jun S. Robust growth of *Escherichia*
587 *coli*. *Current biology*. 2010; 20(12):1099–1103.

588 [29] **Zhang P**, Kaushik AM, Hsieh K, Li S, Lewis S, Mach KE, Liao JC, Carroll KC, Wang
589 TH. A Cascaded Droplet Microfluidic Platform Enables High-Throughput Single Cell Antibiotic
590 Susceptibility Testing at Scale. *Small Methods*. 2022; 6(1):2101254. <https://onlinelibrary.wiley.com/doi/abs/10.1002/smtb.202101254>, doi: 10.1002/smtb.202101254, _eprint:
591 <https://onlinelibrary.wiley.com/doi/pdf/10.1002/smtb.202101254>.

592

593 [30] **Zhou W**, Le J, Chen Y, Cai Y, Hong Z, Chai Y. Recent advances in microfluidic devices for bacteria and fungus research. *TrAC Trends in Analytical Chemistry*.
594 2019; 112:175–195. <https://www.sciencedirect.com/science/article/pii/S0165993618305193>, doi:
595 <https://doi.org/10.1016/j.trac.2018.12.024>.
596