

1 **A standardized head-fixation system for performing large-**

2 **scale, *in vivo* physiological recordings in mice**

3

4 Groblewski PA^{1,3}, Sullivan D^{1,3}, Lecoq J¹, de Vries SEJ¹, Caldejon S¹, L'Heureux Q¹, Keenan T²,
5 Roll K¹, Slaughterback C¹, Williford A¹, Farrell C¹

6 1. Allen Institute for Brain Science, Seattle, WA 98109, USA

7 2. Current Address: Amazon Logistics, Bellevue, WA 98004, USA

8 3. Co-lead authors

9 4. Correspondence: peterg@alleninstitute.org

10 **ABSTRACT**

11 The Allen Institute recently built a set of high-throughput experimental pipelines to collect
12 comprehensive *in vivo* surveys of physiological activity in the visual cortex of awake, head-fixed
13 mice. Developing these large-scale, industrial-like pipelines posed many scientific, operational,
14 and engineering challenges.

15 Our strategies for creating a cross-platform reference space to which all pipeline datasets were
16 mapped required development of 1) a robust headframe, 2) a reproducible clamping system,
17 and 3) data-collection systems that are built, and maintained, around precise alignment with a
18 reference artifact.

19 When paired with our pipeline clamping system, our headframe exceeded deflection and
20 reproducibility requirements. By leveraging our headframe and clamping system we were able
21 to create a cross-platform reference space to which multi-modal imaging datasets could be
22 mapped. Together, the *Allen Brain Observatory* headframe, surgical tooling, clamping system,
23 and system registration strategy create a unique system for collecting large amounts of
24 standardized *in vivo* datasets over long periods of time. Moreover, the integrated approach to
25 cross-platform registration allows for multi-modal datasets to be collected within a shared
26 reference space.

27 Here we report the engineering strategies that we implemented when creating the *Allen Brain*
28 *Observatory* physiology pipelines. All of the documentation related to headframe, surgical
29 tooling, and clamp design has been made freely available and can be readily manufactured or
30 procured. The engineering strategy, or components of the strategy, described in this report can
31 be tailored and applied by external researchers in order to improve data standardization and
32 stability.

33

34 **INTRODUCTION**

35 One of the overarching goals of the Allen Institute for Brain Science is to deepen our
36 understanding of the mammalian visual system, from the moment at which photons enter the
37 eyes to the execution of complex visually guided behavior (Koch & Reid, 2012). To achieve this
38 goal we have constructed the *Allen Brain Observatories* to collect comprehensive maps of
39 neural activity in awake behaving mice. These large-scale efforts will yield complementary
40 optical physiology, electrophysiology, and behavioral datasets of unprecedented size and
41 standardization—all of which will be made freely available to the scientific community for
42 continued analysis. Performing the experiments necessary to collect these datasets posed
43 significant operational and engineering challenges. Here we describe the unique difficulties of,
44 and our solutions for, collecting systematic physiological data from head-fixed mice at scale.

45 The *Allen Brain Observatory* pipelines are composed of a diverse set of experimental
46 platforms—each of which consisted of between 2 and 24 identically constructed instruments
47 operated by teams of technicians. Pipeline platforms include 1) surgical photo-documentation,
48 2) intrinsic signal imaging (ISI), 3) behavioral training, and 4) optical or electrophysiology (de
49 Vries et al., 2019; Siegle et al., 2019). A fundamental requirement of these pipelines was that
50 each instrument needed to be built and operated around a head-fixed mouse such that the
51 position of an individual mouse's eye with respect to the visual stimulus monitor was consistent

52 over many sessions/days, as well as across all data-collection platforms (and instruments within
53 each platform).

54 The operational and scientific requirements of the *Allen Brain Observatory* necessitated
55 a comprehensive engineering strategy to ensure the stability and quality of datasets that were
56 collected by teams of technicians over long-periods of time. Our strategy was to create a
57 “cross-platform reference space” by defining and fully constraining datum structures on mating
58 components—both in rotation and translation. This reference space is defined by the three
59 mutually intersecting perpendicular datum planes created upon immobilization of the headplate
60 within the clamp. Critically, this reference space allows for spatial information to be defined and
61 translated both within and between platforms. Furthermore, it allows consistent placement of all
62 experimental components and instrumentation relative to the reference space and therefore to
63 the mouse.

64 The fundamentals of a cross-platform reference space are based on the definition of a
65 shared Cartesian coordinate space that is referenced to known biological features; in this case
66 we relied on common mouse skull fiducials including lambda, bregma, and the interaural line.
67 There are three components that are necessary for creating a shared coordinate space for data
68 collected from hundreds of head-fixed mice using many instruments: 1) a robust headframe, 2)
69 a reproducible clamping system, and 3) data-collection systems that are built, and maintained,
70 around precise alignment with a reference artifact.

71 Here we describe in detail the engineering strategies and tools we implemented to build
72 and maintain the *Allen Brain Observatory* pipelines. Our strategy for melding standardization
73 with scale was to create an experiment-wide coordinate system, or cross-platform reference
74 space. The cross-platform reference space required designing and validating a suite of
75 equipment and tools, which we describe below and are being made freely available as an open
76 resource to the scientific community.

77

78 RESULTS

79 The first engineering challenge that we faced in building a cross-reference space for the
80 *Allen Brain Observatory* pipelines was to design a robust headframe. Together with our
81 scientific and operational teams we defined the following headframe requirements:

- 82 1. Registrability and rigidity: the headframe needed be rigid (no more than 4 μ m of
83 deflection) and registerable across various instruments, allowing for a single set of cells
84 to be recorded by multiple instruments over many experimental sessions.
- 85 2. Basic geometrical and experimental constraints: the headframe and well needed to be
86 compatible with our various pipeline instruments and allow for physiological recording
87 access to all visual cortical regions.
- 88 3. Animal health: the headframe needed to be lightweight (no more than 10% of
89 bodyweight), made of biocompatible material, and not impair normal in-cage mouse
90 behavior (including locomotion, feeding and drinking).
- 91 4. Ease of handling: head-fixation needed to be easy and quick, thereby reducing
92 unnecessary stress on the animal and experimenter.
- 93 5. Adaptability: the headframe and clamp design needed to be adaptable to other types of
94 physiological recordings from various brain regions.

95 We performed an assessment of the current (as of 2014) state of the art including
96 designs used by various laboratories (e.g. Andermann et al., 2010; Guo et al., 2014) as well as
97 commercially available options (e.g., <https://www.neurotar.com/>). We determined that none of
98 these individual headframe designs satisfied all of our requirements. For instance, most existing
99 headframes required two holding clamps—a design that would force the system to be statically
100 indeterminate, thereby preventing knowledge of exact headframe location (and thus any cells of
101 interest) as well as placing physical strains on the headframe. Furthermore, most headframe
102 clamp interfaces lacked constrainable datum structures necessary to remove rotational and
103 translational degrees of freedom (required for reproducible placement of the headframe on the
104 skull, as well as registration across instruments/platforms). Upon assessment of existing
105 headframes, we decided to create a novel design, which allowed us to incorporate all the
106 necessary features from the ground up. While iterating on the headframe design we co-
107 developed a surgical procedure and set of custom surgical tooling that would precisely place the
108 headframe relative to the mouse skull. (See *Headframe and Headframe Surgical Tooling*)

109 The second requirement of a cross-platform reference space is a robust clamping
110 system and for this we relied on a clamping interface that we had incorporated into the
111 headframe shank. The headframe's built-in registerable faces/features allowed it to be
112 reproducibly placed and secured into the clamps of the various instruments. (See *Clamping*
113 *System & System Alignment*)

114 The final requirement of the cross-platform reference space is that the data collection
115 systems are designed, built and maintained around precise alignment with a single reference
116 artifact; we used a reticle. An important challenge that we faced was that the pipeline platforms
117 are diverse and possess unique sets of constraints related to both the mode of data acquisition
118 (e.g. ISI camera vs 2-photon microscope objective) and physical attributes (including size,
119 shape, and orientation). To standardize mouse placement across these diverse platforms we
120 created hardware solutions that incorporated a common mouse stage that placed mice at a
121 fixed geometry with respect to the visual stimulus monitor (Supplemental Figures 1, 3, and 4).
122 Importantly, these features are set and validated independently of biological variation and permit
123 long-term monitoring of system alignment. (See *Systems & Applications and Cross-Platform*
124 *Registration*)

125 **Headframe**

126 DESIGN: The headplate design and dimensions are shown in the plan and side views
127 of Figure 1a, and isometric views of Figure 1b. The headplate comprises two main parts: a
128 shank (the feature that is loaded into a clamp) and the mouse-interface that, in this case,
129 encircles the visual area of the cortex in the left hemisphere (see below for stereotaxic
130 coordinates).

131 The shank design includes three perpendicular, manufactured surfaces that define a
132 datum reference frame (shown as A, B, and C in Figure 1a). The reference frame on the
133 headplate mates to the corresponding reference frame on the clamp of each instrument and
134 constrains the three translational (x, y, z) and three rotational (pitch, roll, yaw) degrees of
135 freedom. The common reference frame provides a physical origin point to which all visual
136 stimuli and instrumentation are placed in three-dimensional space. Incorporating the physical
137 origin point in the design of each of our instruments ensures that the mouse experiences the
138 same stimulus across every platform (and every instrument within each platform) of the pipeline.

139 The design of the mouse interface of the headplate was driven by 1) the area of interest
140 for physiological recordings, 2) the microscope or other instrument interface, and 3) the
141 geometry of the mouse skull. The headframe developed for the *Allen Brain Observatory*
142 consists of a 10 mm circular opening centered over the putative location of the primary visual
143 cortex (M/L= -2.8 mm, A/P = 1.3 mm, with respect to lambda). The 10 mm ring features a slight
144 teardrop shape to accommodate skull variation between animals and provides clearance for a
145 more reproducible, unobstructed skull contact point across mice. The headplate is mated to a
146 water-retention well that was designed to interface with a 16X Nikon CFI LWD Plan Fluorite
147 Objective. It's important to note, that the design of the mouse interface and well are easily
148 adaptable to other regions of the mouse skull (to gain access to other brain structures of
149 interest), other objectives or instruments, and/ other surgical preparations, all while retaining the
150 datum reference frame of the shank and its placement relative to the three biological features.

151 A final requirement of the headplate was that it should provide a finger-hold to help ease
152 the clamping procedure for head-fixation. The 'd-loop', visible in Figures 1a and b, fulfills this
153 need without adding significant weight, requiring additional handling tools, or obstructing the
154 mouse's view of the stimulus monitor.

155 **ANIMAL HEALTH REQUIREMENTS:** The *Allen Brain Observatory* headplate is
156 manufactured from 6Al-4V titanium using common manufacturing methods (see *Materials &*
157 *Methods*). Titanium's biocompatibility is well understood and, as such, it is often selected for
158 implants in mice and humans (Sidambe, 2014). Given its desirable stiffness-to-weight ratio it is
159 an especially good fit for this application and is routinely used for similar *in vivo* neuroscience
160 applications (e.g., Guo et al., 2014; Hefendehl et al., 2012). The finished headplate mass is
161 ~1.9 g (approximately 10% of body weight of a minimum weight mouse at the time of
162 implantation). We monitored in-cage behavior of mice following surgery and observed that mice
163 can eat, drink, and locomote normally with the headframe and well attached to the skull.

164 **EXPERIMENTAL REQUIREMENTS:** The experimental paradigm requires that, to the
165 greatest extent possible, the mouse's view of the stimulus screen is unobstructed. The visual
166 field of the right eye extends approximately to 110 degrees vertical, 140 degrees horizontal
167 (Wagor et al., 1980) while the stimulus monitor extends to +/-47 degrees in the vertical and +/-
168 59.3 degrees in the horizontal from the gaze axis of the mouse. To keep the visual field clear,
169 the shank of the headplate was kept to the rear of the skull and was also raised above the body
170 of the mouse to keep it clear of the neck and back (that is, it is parallel to and elevated from the
171 x-y plane of the mouse coordinate system) (Figure 1b).

172 As one of the experimental requirements for our headpost design, our 2P microscopy
173 team determined *a priori* that the imaging region of interest must exhibit no more than 4 μ m of
174 total displacement along the optical axis during an experiment. Figure 2a shows the results of a
175 computer simulation to assess how the headframe and clamp performed under a downward, 0.5
176 N load distributed across the entire ring of the headplate. We deemed a 0.5 N force to be a
177 conservative estimate when compared to an average running mouse with mass of
178 approximately 20 grams (0.196 Newtons) without the ability to exert significant force on a low
179 stiffness, foam-covered running disk. The simulations showed that the 0.5 N load resulted in a
180 displacement of approximately 1.5-2 μ m at the center of the ring, with a maximum deflection of
181 ~3 μ m at the outer edge of the ring. Figure 2b shows the results of our bench tests during
182 which we measured the actual deflection (measured at ring center and rim using a laser
183 displacement sensor) caused by 20 g, 50 g, and 100 g weights hung under the outer rim of the

184 headplate ring. Our tests confirmed that the titanium headpost, coupled with our pipeline
185 clamping mechanism, demonstrated an average of 3.2 μm of displacement at the center of the
186 ring under a static 0.49 N (50 g) load applied to the far end of the headplate. A final set of tests
187 were performed to assess the deflection of the headframe and cranial window surface in actual
188 mice. Specifically, following recovery from the Headframe & Cranial Window surgery (see
189 *Materials & Methods*) two mice were head-fixed in a pipeline 2P microscope instrument and
190 deflection measurements were obtained while the mice were actively locomoting (i.e., during
191 bouts of running and stopping). The results of these tests are shown in Figure 2c, overlaid with
192 a baseline measurement of noise. As expected, there was minor displacement of the
193 headframe when the mice were locomoting and this displacement increased slightly when
194 measured at the surface of the cranial window (as indicated in the example traces and
195 histograms, as well as reflected by the increase in signal variance). Importantly, however,
196 maximum displacement ($\leq 2.2 \mu\text{m}$), and even total range of displacement during the entire
197 recording period ($\leq 3.3 \mu\text{m}$), was well within our experimental tolerances.

198 ***Headframe Surgical Tooling***

199 The *Allen Brain Observatory* cranial window surgery has previously been described in
200 detail (de Vries et al., 2019) as well as in the *Materials & Methods*. Additional information can
201 be found at <https://help.brain-map.org/display/observatory/Documentation>.

202 **HEADFRAME PLACEMENT:** To standardize the placement of the headframe onto the
203 mouse skull we designed a custom set of tools that remove all angular degrees of freedom, as
204 well as X and Y variability, from the headframe installation process. These tools include a
205 “headframe clamp” and “stylus”. The “headframe clamp” tool interfaces with KOPF Model
206 #1900 dovetail mounts and suspends a clamshell-style clamp above the mouse. Once the
207 mouse’s skull is levelled with respect to pitch (bregma-lambda level), roll, and yaw, the
208 “headframe clamp” tool is secured in the KOPF arm and aligned so that the clamp is positioned
209 at a known offset from lambda (the coordinate system origin). This is achieved with the custom
210 “stylus”, shown in Figure 3a. The “stylus” tool shares the same shank as the headplate and so
211 utilizes the same datum registration surfaces. It is installed in the “headframe clamp” tool
212 (Figure 3b) and the surgeon adjusts the X and Y axes of the stereotaxic instrument to locate the
213 tip of the “stylus” at lambda. Once lambda is located, the “stylus” is removed from the clamp
214 and a headframe is installed and lowered until the anterior portion of the headplate contacts the
215 skull. The headframe is cemented to the skull and once dry, the clamshell is opened, releasing
216 the headframe. This tool reproducibly places the headframe such that the center of the well is
217 precisely 2.8 mm lateral and 1.3 mm anterior to lambda (Figure 3a).

218 **CRANIOTOMY & CRANIAL WINDOW:** To facilitate repeatable location of the
219 craniotomy and cranial window we designed a custom clamp pictured in Figure 3c. The
220 “levelling clamp” was designed to fit into the KOPF Model #1900 earbar holder upon removing
221 the right earbar and is compatible with the anesthesia nose cone (although the mouse must be
222 removed from the bite bar clamp). The “levelling clamp” has a built-in forward pitch of 6°, and
223 along with rotation of the entire earbar apparatus to a roll angle of 23° (using a custom-adapted
224 angle finder not pictured) it holds the craniotomy plane perpendicular to gravity. Once the
225 headframed animal is clamped and rotated, a circular piece of skull (5 mm in diameter) is
226 removed with a dental drill, and a durotomy is performed. The “levelling clamp” facilitates drilling
227 of the craniotomy (and subsequent durotomy) by 1) allowing the surface of the skull (and 2)
228 subsequently the brain) to be more clearly viewed through the stereo microscope and 2)

229 keeping artificial cerebrospinal fluid used during the procedure contained within the headplate
230 ring. Following the craniotomy and durotomy, a 0.45 mm thick custom borosilicate glass
231 coverslip (stacked appearance with a 5 mm diameter “core” and 7 mm diameter “flange”) is
232 cemented in place. The “leveling clamp” facilitates consistent placement and cementing of the
233 cranial window at an angle that is approximately parallel to the headplate ring, and thus normal
234 to the imaging axis of our pipeline data-collection instruments.

235 ***Clamping System & System Alignment***

236 **CLAMP DESIGN:** To accurately place the animal relative to stimulus monitor and
237 instrumentation (e.g., the microscope objective) we developed a custom clamping mechanism
238 shown in Figure 4. This clamping mechanism simultaneously meets multiple requirements
239 including 1) robust reproducibility, 2) high stiffness, 3) quick installation and removal with
240 common tools, and 4) compatibility with all *Allen Brain Observatory* platforms. An additional
241 design requirement was that the clamping mechanism be manufactured with commonly
242 available screws, materials, and processes. The clamp was designed to position the headplate
243 shank into the common datum surface with two, screw-driven mechanisms pushing
244 perpendicular to each other and at 45 degrees with respect to the planes they are pushing
245 against (see Figure 4a). The headplate is inserted, and positively located into the corner of the
246 clamp and it can be installed or released in under 10 seconds (Figure 4b). An optional third
247 screw (Figure 4b) is utilized for applications demanding the utmost stability of the animal (e.g.,
248 2P microscopy). The datum surfaces of the headplate and clamp are broad to prevent wear,
249 while the force application points can accommodate manufacturing variation and wear without
250 sacrificing clamping accuracy. It is important to note that accuracy is highly dependent on clean
251 reference surfaces; buildup of dirt, debris and animal dander will impact clamping accuracy and,
252 therefore, headplate cleanliness must be maintained throughout the duration of
253 experimentation.

254 **SYSTEM ALIGNMENT:** Despite possessing common mouse-to-screen geometry
255 (depicted in Supplemental Figure 1a), each of the *Allen Brain Observatory* data-collection
256 systems possessed slightly different rotational, translational, and scaling attributes of image
257 acquisition. To accommodate inter-instrument variability in these image attributes, we
258 employed a registration artifact in the form of a reticle that incorporated the geometry and
259 clamping interface of the experimental headframe (Figure 5a). Importantly, the reticle was
260 mounted in the headframe at approximately the imaging depth of interest. Instrument-specific
261 reticle images were obtained, and exact positioning was monitored over time to ensure
262 consistent system registration (see *Systems & Applications*).

263 It is worth noting that alignment of a small number of instruments can be performed with
264 a single reticle. However, in our case we implemented a second layer of abstraction wherein
265 instruments are registered to a platform-specific, secondary reticle. Each of the secondary
266 reticles is registered to a single primary reticle. Thus, images obtained on an instrument were
267 translated to a common primary coordinate space using that instrument’s platform’s secondary-
268 to-primary set of translation values. A two-layer reticle system allowed us to independently
269 maintain alignment of 40+ instruments across 4 platforms without having to rely on a single
270 reticle.

271 ***Systems & Applications***

272 **SURGICAL PHOTO-DOCUMENTATION:** Post-surgical brain health and window clarity
273 were documented using a custom surgical photo-documentation system (in addition to normal
274 animal health checks at one, two, and seven days following surgery). The photo-documentation
275 apparatus (Supplemental Figure 2a) was custom designed to provide a registered image of the
276 cranial window using the standard pipeline geometry (Supplemental Figure 1a). Because mice
277 were imaged at the end of surgery, they were still lightly anesthetized and, as such, there was
278 no need to include the third screw in the clamping mechanism. Additionally, because there was
279 no visual stimulation for this data-collection step, the system did not include a stimulus screen.

280 Each of two photo-documentation systems were initially registered, and subsequently
281 monitored weekly, by analyzing images of a secondary reticle. A sample of 18 months of
282 longitudinal registration monitoring data is shown in Figure 5b. Repeated detections of >22.5
283 μm deviation from the registered reticle location triggered system re-registration (shown as
284 colored hash marks). The median of monitoring data for each system was calculated and
285 indicated a clamping variability of 10.61 μm for these systems.

286 **INTRINSIC SIGNAL IMAGING:** The *Allen Brain Observatory* pipelines utilize intrinsic
287 signal imaging (ISI) with every mouse for targeting physiology recordings. Briefly, ISI measures
288 the hemodynamic response of the cortex to visual stimulation across the entire field of view in
289 mice that are lightly anesthetized. This retinotopic map effectively represents the spatial
290 relationship of the visual field to locations within each cortical area. Retinotopic mapping is
291 used to delineate functionally defined visual area boundaries and enable targeting of the *in vivo*
292 physiology to retinotopically defined locations in primary and secondary visual areas (Garrett et
293 al., 2014).

294 The ISI instruments had a different mouse-to-screen geometry (compared to the other
295 pipeline platforms) and comprised an Andor Zyla 5.5 sCMOS camera and a ring illumination
296 system of independently controlled green and red LEDs (Supplemental Figure 2b). The camera
297 was fixed normal to the nominal window pitch and roll (6° and 23°, respectively). In addition to
298 the camera and stimulus screen, the ISI system was equipped with an anesthesia machine
299 (SomnoSuite, Torrington, CT) that was used to maintain a light plane of anesthesia during the
300 ISI session. Because mice were lightly anesthetized there was no need to include the third
301 screw in the clamping mechanism. As with the surgical photo-documentation system, each of
302 three ISI systems were monitored for registration using a secondary reticle. A sample of 24
303 months of longitudinal monitoring is shown in Figure 5c. Colored hash marks on the x-axis
304 indicate when the different systems required re-registration (due to reticle measurements drifting
305 more than 22.5 μm from the original location). The median for each system indicated ISI
306 clamping variability ranging from 4.5 to 11.25 μm.

307 **BEHAVIOR:** To support multiple versions of the *Allen Brain Observatory* we designed
308 and built a large-scale behavior training facility that could simultaneously accommodate the
309 behavior-training requirements of multiple pipelines. Each of these mouse behavior training
310 enclosures (24 in total) were identically built to maintain the standard pipeline mouse-screen
311 geometry.

312 The engineering requirements for the behavior platform included 1) a compact, modular
313 design that allowed for training of ~100 mice per day, 2) the ability to perform several different
314 behavior tasks in different enclosures concurrently, 3) easy and reproducible clamping, and 4)
315 pipeline mouse-screen geometry. Supplemental Figure 3a shows a front view of a behavior
316 enclosure equipped with stimulus screen, sound-attenuating foam, ventilation fan, and a fixed-

317 location camera (Allied Vision, Mako G-032B) to continuously monitor mice while in the
318 enclosure. Mice are head-fixed on a removable behavior stage equipped with a running disc
319 (Supplemental Figure 3b) and then placed onto a kinematic mount in the behavior enclosure,
320 thereby ensuring quick but reproducible placement of the mouse with respect to the screen.

321 **IN VIVO, 2-PHOTON CALCIUM IMAGING:** The first iteration of the *Allen Brain*
322 Observatory pipeline consisted of *in vivo* 2P calcium imaging in awake mice over multiple
323 sessions/days. Our pipeline data collection systems were built around two off-the-shelf
324 microscope models, Scientifica Vivoscope or Nikon A1R MP+, that we modified to
325 accommodate our scientific and engineering requirements for pipeline data collection. In
326 addition to incorporating our behavior stage (with running disc) and stimulus screen (ASUS
327 PA248Q), each system was equipped with eye-tracking and full-body cameras (Allied Vision,
328 Mako G-032B), each with their own LED illumination source. Both the Nikon and Scientifica
329 systems are shown in Supplemental Figure 4.

330 The engineering requirements for the 2P calcium imaging platform were the most
331 stringent and included 1) the ability to navigate to the same 400 x 400 μm field of view (and thus
332 the same neurons) over multiple sessions/days, 2) a stable, rigid headframe and clamping
333 system that allowed for no more than 4 μm of flex along the optical axis, and 3) pipeline mouse-
334 screen geometry. Clamping performance was tested and the results of these tests is reported
335 below.

336 ***Cross-Platform Registration***

337 As mentioned previously, to accommodate inter-instrument variability, we employed a
338 reticle registration procedure that ensured initial system alignment as well as maintenance of
339 that alignment over time. Precise reticle alignment had the added benefit that image capture
340 from a diverse set of platforms could be translated to, and compared within, a shared coordinate
341 space through a series of rotational, axial, and scaling factors. Specifically, each instrument
342 had an established set of translation values to a platform-specific secondary reticle (obtained
343 during system alignment, monitored, and updated if necessary), and each secondary reticle had
344 a known set of different translation values to a common, primary reticle. As such, images
345 obtained with any of our pipeline instruments could be translated to a common image space,
346 resulting in “cross-platform registration” (Figure 6a).

347 The *Allen Brain Observatory* pipelines utilize ISI maps obtained from each individual
348 mouse to perform physiological recordings in precise, retinotopic locations within the visual
349 cortex. Because the instruments of the ISI and 2P microscopy platforms were all registered to a
350 common reference space, we were able to identify the coordinates of a retinotopically-defined
351 region (referenced to the ISI home location), translate the coordinates to the 2P reference
352 space, and then drive to the target recording location from the 2P home location (Figure 6b).
353 Accuracy of the ISI-2P translation in a non-biological sample is depicted in Figure 6c, which
354 shows the trial-to-trial variability of navigating to a set of five ISI-translated coordinates (red
355 crosses) on various 2P microscopes. Across three pipeline 2P instruments, targeting was 10-50
356 μm (median = 37.6 μm , sd = 9.93) off from the desired location, where factors contributing to
357 this variability included clamping and coordinate translation.

358 In an experimental setting, however, there are additional biological factors that can
359 impact targeting accuracy, including brain motion. Prior to each 2P recording session,
360 operators were able to make an adjustment of the 2P home location so that it matched the ISI

361 home location; this was performed in epifluorescence mode with 800 μ m field of view (FOV).
362 This “home offset” was then applied to the translated X and Y coordinates of the target
363 recording location chosen from the ISI map. In a sample of our pipeline experiments (1712
364 sessions), the “home offset” adjustment values ranged from 0 to 905 μ m, with median values of
365 74 μ m and 57 μ m in X and Y, respectively (Figure 6d). As previously mentioned, this
366 adjustment accounted for variability caused by brain motion and was often necessary in order to
367 adjust for any tissue motion that had occurred since the ISI, or previous 2P, session.

368 After navigating to the target recording site using the translated ISI coordinates, the
369 operator was able to make final adjustments to the 400 μ m, 2P FOV to ensure optimal cell
370 matching with previous recording sessions. Figure 6e shows the day-to-day FOV targeting
371 results from a sample of pipeline experiments (5 experiments with an average of 9.5 imaging
372 sessions per experiment). Specifically, median adjustments of 16.47 μ m (in X) and 16.34 μ m
373 (in Y) were required to match the 400 x 400 μ m imaging FOV across sessions/days once the
374 initial target FOV had been set on the first recording session. These adjustments account for
375 variability in cell movement, stage movement, and translation from epifluorescence to 2P. To
376 further illustrate the accuracy of these systems, the median X and Y adjustments are again
377 shown referenced to an example 2P FOV of GCaMP6+ neurons in the visual cortex (Figure 6e,
378 right). In all, these systems exhibited variability well within our tolerances for performing
379 experiments targeted at a single set of cells across many sessions/days.

380

381 DISCUSSION

382 In order to build the *Allen Brain Observatory* pipelines capable of collecting standardized
383 datasets from head-fixed mice over long-periods of time we developed a series of integrated
384 experimental platforms, each consisting of instruments that were built and registered to a
385 shared coordinate space. Our cross-platform reference space strategy was based not only on
386 creating a headframe and clamping systems, but also developing associated standard operating
387 procedures for operation and routine monitoring and maintenance.

388 Creating a cross-platform reference space for our pipeline systems required three
389 essential components: 1) a robust headframe, 2) a reproducible clamping system, and 3) data-
390 collection systems that are built, and maintained, around precise alignment with a reference
391 artifact. Additionally, the design of our pipeline systems had to meet the scientific requirements
392 of our experimental goals and the teams of technicians who were responsible for operating the
393 systems. Here we have described our head-fixation strategies for meeting the engineering,
394 scientific, and operational requirements of our large-scale, *in vivo* pipelines.

395 We developed a headframe and a set of surgical tools and procedures for reproducibly
396 affixing the headframe to the mouse utilizing a set of skull fiducials. The headframe design
397 incorporated features that created three mutually intersecting perpendicular datum planes and,
398 when affixed to mice using our surgical tooling and procedures, allowed for precise placement
399 of mice across all of our various experimental instruments. Although our headframe was
400 designed for our specific scientific goals, the mouse-interface portion (and associated surgical
401 tooling) can easily be redesigned to accommodate alternative experimental modalities and/or
402 recordings in other brain regions. Importantly, this can be done while still maintaining the
403 mouse-to-screen geometry, which is accomplished by maintaining the design of the shank and

404 its relationship to the skull fiducials. For example, we have adapted the Brain Observatory 2P
405 headframe to gain access to more lateral visual areas as well as accommodate use of our multi-
406 plane, Mesoscope imaging platform and objective (Supplemental Figures 5a and b,
407 respectively). Additionally, we have adapted our headframe to accommodate different recording
408 modalities including multi-probe electrophysiology, through-skull widefield imaging, and
409 electroencephalogram (EEG) arrays (Supplemental Figures 5c-e).

410 To integrate our head-fixation system into the *Allen Brain Observatory* pipeline we built a
411 series of multi-modal data-collection systems that were all precisely aligned to a reference
412 reticle. The precise alignment of these systems, and our ability to closely monitor alignment
413 over time, allowed us to register our pipeline datasets across experimental platforms and
414 leverage this registration for large-scale data collection. Here we report that these systems
415 remain stable over long periods of time and frequent use and can be easily re-registered if
416 deviations occur. Additionally, we describe an experimental application of cross-platform
417 registration, made possible by our head-fixation system paired with routine system monitoring.

418 Since building the initial *Allen Brain Observatory* pipeline we have expanded the
419 application of our engineering strategy to various other pipelines that utilize other recording
420 modalities. Specifically, we extended the visual coding 2P pipeline to include a multi-depth 2P
421 microscopy platform (Liu et al., 2019) as well as a multi-area/depth Neuropixels platform that is
422 capable of recording from 6 high-density electrophysiology probes in an awake mouse (Siegle
423 et al., 2019). In addition to our various visual coding pipelines, we have more recently built 3
424 visual behavior pipelines that allow for performing single- and multi-plane 2P (Tsybouski et al.,
425 2018), as well as Neuropixels, recordings from head-fixed mice performing visually-guided
426 operant behavioral tasks. Each of the aforementioned *Allen Brain Observatory* pipelines were
427 built around the cross-platform reference space described here and thus all meet our scientific
428 and engineering requirements. In addition to the *Allen Brain Observatory* datasets being free to
429 download from our web portal (<https://portal.brain-map.org/explore/circuits>), all files related to
430 the tools and resources described in this report are made freely available via our toolkit portal
431 (<https://portal.brain-map.org/explore/toolkit/hardware>). Although it may not be feasible/desirable
432 for external researchers to adopt our pipeline hardware and procedures in toto, we believe that
433 incorporation of components of our engineering strategy could help to improve standardization
434 and quality of physiology datasets obtained from head-fixed mice.

435

436 MATERIALS & METHODS

437 *Headframe & Clamp Manufacturing*

438 **HEADFRAME:** The headplate is manufactured from nominally 1.6 mm (.063 inch) thick
439 titanium 6Al-4V annealed sheet and processed using common manufacturing methods. The
440 Allen Institute selects material that is on the plus side of the sheet tolerance to prevent clamp
441 adjustments that may be needed when switching between headplates that have thicknesses at
442 the extremes of the tolerance band, which provides a maximum sheet thickness of 1.7mm (.068
443 inch). The raw sheet is waterjet cut, and the parts are tumble-deburred before being formed in
444 a jig to add the correct angle for the mouse-interface. To prevent cracking during forming the
445 component is heated slightly above room temperature to between 50 C and 100 C. Headplate
446 manufacturing variances are kept to +/- 0.1 mm or better on all dimensions to ensure balance of

447 manufacturability and compatibility with the clamping system, maintain consistency throughout
448 the lifetime of the experiment, and to allow high precision placement of the headplate on the
449 animal. It is worth noting that for smaller scale experimentation, headframes can be produced
450 with 3D printing, without any compromises to datum surface registration or rigidity (Karolewska
451 & Ligaj, 2019; Owsinski & Nieslony, 2018). Additionally, if so desired, titanium headframes can
452 be removed from mice post-mortem, cleaned, and reused.

453 **CLAMP:** The custom-designed clamping system components are all manufactured with
454 common materials and traditional methods and can be produced on common CNC mills. The
455 fasteners and alignment pins are commercially and commonly available. During assembly,
456 alignment of the side clamp (Figure 4) is performed with custom tooling to ensure accuracy and
457 repeatability of headplate clamping. All other components are pinned and aligned by reference
458 features and no custom tooling is required.

459 ***Headframe Testing***

460 **SIMULATION:** Design of the headframe and clamping systems were guided by
461 assumptions on loading and the amount of mass a mouse could reasonably carry as an implant.
462 With these basic assumptions the design effort proceeded with a goal to maximize stiffness of
463 the headplate, while limiting the implant weight to 2 grams. Loads imparted into the system by a
464 head-fixed behaving mouse were estimated to be at most .5N, or roughly an average weight
465 mouse accelerating at 2 g vertically. External mechanical inputs were deemed to be negligible.

466 To compare designs and materials a static linear analysis was developed in Solidworks
467 Simulation (Solidworks, Dassault Systemes). This simulation is founded on the “finite element
468 method” and allows loads, supports and material behaviors to be realistically simulated when
469 loaded in the linear elastic strain range of the materials involved, which is valid in this scenario.
470 For this model an external vertically oriented load of 0.5N was distributed along the interior rim
471 of the headplate (consistent with physical attachment to the mouse) and the clamp was
472 constrained to zero motion at its fastener attachments. The headplate is modeled so as to be
473 constrained to the clamp at the datum interfaces (Figure 1a). A solid mesh with approximately
474 1mm nominal element size was chosen to allow fine displacement detail to be resolved in the
475 thin headplate and is well beyond the mesh density necessary to obtain results convergence.

476 The model was used to study and compare a variety of clamp and headplate materials
477 including implantable plastics, aluminum, carbon fiber, stainless steels and titanium. The
478 resulting design selected titanium 6Al-4V for the headplate and stainless steel 304 for the main
479 clamping body. Results of this simulation are shown in Figure 2a and agrees well with bench
480 testing of the loaded headplate as shown in Figure 2b.

481 **BENCH TESTING:** Bench deflection testing was performed using a Micro Epsilon laser
482 triangulation displacement sensor, ILD1750-10 with a repeatability of 0.4 μ m, a spot size of 110
483 μ m and a range of 10mm. The instrument was placed within range, normal to the headplate at
484 various testing locations. A static load was applied with calibrated weights freely hanging from
485 the headplate from a small wire hook. The load was applied and released 3 times for a variety
486 of different load scenarios and points of interest and is summarized in Figure 2b.

487 **IN VIVO TESTING:** Final deflection tests were performed on awake, locomoting mice
488 that were head-fixed in our pipeline 2P microscope’s clamping system (Figure 2c). A Micro
489 Epsilon sensor was used to first record baseline noise by recording deflection of a headframe

490 alone (no mouse) clamped into the system (“Baseline”). Deflection was then assessed in 2
491 different mice that wereby obtaining multiple 20s recordings from the headframe surface
492 (“MouseX_HF”) as well as from the surface of the cranial window (“MouseX_Win”).

493 **Surgery**

494 All experiments and procedures were performed in accordance with protocols approved
495 by the Allen Institute Animal Care and Use Committee. Headpost and cranial window surgery
496 was performed on healthy male and female transgenic mice (p37-p63) weighing no less than 15
497 g at time of surgery and was based on a previously published protocol (Goldey et al., 2014).
498 Pre-operative injections of dexamethasone (3.2 mg/kg, S.C.) were administered at 12h and 3h
499 before surgery. Mice were initially anesthetized with 5% isoflurane (1-3 min) and placed in a
500 stereotaxic frame (Model# 1900, KOPF; Tujunga, CA), and isoflurane levels were maintained at
501 1.5-2.5% for surgery. An incision was made to remove skin, and the exposed skull was levelled
502 with respect to pitch (bregma-lambda level), roll and yaw. The stereotax was zeroed at lambda
503 using a custom headframe holder equipped with stylus affixed to a clamp-plate (see *Headframe*
504 *Surgical Tooling*). The stylus was then replaced with the headframe to center the headframe
505 well at 2.8 mm lateral and 1.3 mm anterior to lambda. The headframe was affixed to the skull
506 with white dental cement (C&B Metabond; Parkell; Edgewood, NY) and once dried, the mouse
507 was placed in a custom clamp to position the skull at a rotated angle of 23° such that the visual
508 cortex was horizontal to facilitate creation of the craniotomy (see *Headframe Surgical Tooling*).
509 A circular piece of skull 5 mm in diameter was removed, and a durotomy was performed. A
510 glass coverslip (cut from a single piece of glass to obtain a “stacked” appearance that consisted
511 of a 5 mm diameter “core” and 7 mm diameter “flange”), was cemented in place with Vetbond
512 (3M; St. Paul, MN). Cement was then applied around the cranial window inside the well to
513 secure the glass window. Post-surgical brain health was documented using a custom photo-
514 documentation system and animals were assessed one, two, and seven days following surgery
515 for overall health (bright, alert and responsive), cranial window clarity and brain health.

516

517 **ACKNOWLEDGEMENTS**

518 We thank Michael A. Buice, Marina Garrett, Leonard Kuan, Shawn Olsen, Carol
519 Thompson, Wayne Wakeman, Jack Waters, Derric Williams, Nathalie Gaudreault, Fiona Griffin,
520 Perry Hargrave, Robert Howard, Josh Larkin, Rachael Larsen, Eric Lee, Arielle Leon, Jennifer
521 Luviano, Thuyanh Nguyen, Jed Perkins, Miranda Robertson, Sam Seid, Casey White, Ali
522 Williford, Hongkui Zeng, Amy Bernard, John W. Phillips, R. Clay Reid, and Christof Koch for
523 their intellectual and/or experimental contributions.

524 We thank the Animal Care, Transgenic Colony Management, Lab Animal Services and
525 Neurosurgery & Behavior teams for mouse husbandry, care, and surgery.

526 We thank Allan Jones for providing the critical environment that enabled our large scale
527 team effort. We thank the Allen Institute founder, Paul G. Allen, for his vision, encouragement,
528 and support.

529

530 **DECLARATIONS OF INTEREST:** None

531 **REFERENCES**

532 Andermann, M. L., Kerlin, A. M., & Reid, R. C. (2010). Chronic Cellular Imaging of Mouse Visual
533 Cortex During Operant Behavior and Passive Viewing. *Frontiers in Cellular Neuroscience*,
534 4, 3. <https://doi.org/10.3389/fncel.2010.00003>

535 de Vries, S.E.J.*, Lecoq, J.* , Buice, M.A.* , Groblewski, P.A., Ocker, G.K., Oliver, M., ... Koch,
536 C. (2019). A large-scale, standardized physiological survey reveals functional organization
537 of the mouse visual cortex. *Nature Neuroscience*. [https://doi.org/10.1038/s41593-019-0550-9](https://doi.org/10.1038/s41593-019-
538 0550-9)

539 Garrett, M. E., Nauhaus, I., Marshel, J. H., & Callaway, E. M. (2014). Topography and Areal
540 Organization of Mouse Visual Cortex. *Journal of Neuroscience*, 34(37), 12587–12600.
541 <https://doi.org/10.1523/JNEUROSCI.1124-14.2014>

542 Goldey, G. J., Roumis, D. K., Glickfeld, L. L., Kerlin, A. M., Reid, R. C., Bonin, V., ...
543 Andermann, M. L. (2014). Removable cranial windows for long-term imaging in awake
544 mice. *Nature Protocols*, 9(11), 2515–2538. <https://doi.org/10.1038/nprot.2014.165>

545 Guo, Z. V., Hires, S. A., Li, N., O'Connor, D. H., Komiyama, T., Ophir, E., ... Svoboda, K.
546 (2014). Procedures for behavioral experiments in head-fixed mice. *PLoS ONE*, 9(2).
547 <https://doi.org/10.1371/journal.pone.0088678>

548 Hefendehl, J. K., Milford, D., Eicke, D., Wegenast-Braun, B. M., Calhoun, M. E., Grathwohl, S.
549 A., ... Liebig, C. (2012). Repeatable target localization for long-term in vivo imaging of mice
550 with 2-photon microscopy. *Journal of Neuroscience Methods*, 205(2), 357–363.
551 <https://doi.org/10.1016/j.jneumeth.2011.10.029>

552 Karolewska, K., & Ligaj, B. (2019). Comparison analysis of titanium alloy Ti6Al4V produced by
553 metallurgical and 3D printing method. *AIP Conference Proceedings*, 2077(February).
554 <https://doi.org/10.1063/1.5091886>

555 Koch, C., & Reid, R. C. (2012). Observatories of the mind. *Nature*, 483(7390), 397–398.
556 <https://doi.org/10.1038/483397a>

557 Liu, R., Ball, N., Brockill, J., Kuan, L., Millman, D., White, C., ... Saggau, P. (2019). Aberration-
558 free multi-plane imaging of neural activity from the mammalian brain using a fast-switching
559 liquid crystal spatial light modulator. *Biomedical Optics Express*, 10(10), 5059.
560 <https://doi.org/10.1364/boe.10.005059>

561 Owsiński, R., & Niesłony, A. (2018). Fatigue properties in additive manufacturing methods
562 applying Ti6Al4V. *AIP Conference Proceedings*, 2029(October 2018).
563 <https://doi.org/10.1063/1.5066511>

564 Sidambe, A. T. (2014). Biocompatibility of advanced manufactured titanium implants-A review.
565 *Materials*, 7(12), 8168–8188. <https://doi.org/10.3390/ma7128168>

566 Siegle, J. H., Jia, X., Durand, S., Gale, S., & Bennett, C. (2019). A survey of spiking activity
567 reveals a functional hierarchy of mouse corticothalamic visual areas. 1–53.

568 Tsyboulski, D., Orlova, N., Griffin, F., Seid, S., Lecoq, J., & Saggau, P. (2018). Remote focusing
569 system for simultaneous dual-plane mesoscopic multiphoton imaging. *BioRxiv*, 887(2008),
570 503052. <https://doi.org/10.1101/503052>

571 Wagor, E., Mangini, N. J., & Pearlman, A. L. (1980). Retinotopic organization of striate and
572 extrastrate visual cortex in the mouse. *Journal of Comparative Neurology*, 193(1), 187–
573 202. <https://doi.org/10.1002/cne.901930113>

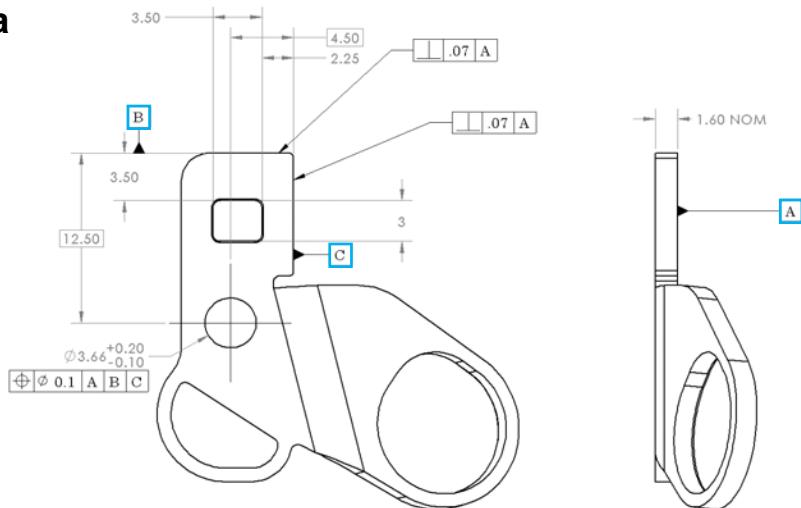
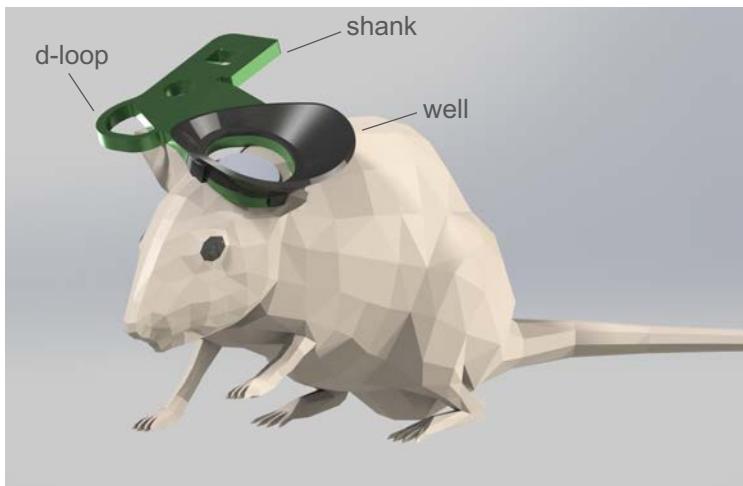
a**b**

Figure 1. Brain Observatory headframe

a) Plan- and side-view of the Brain Observatory headplate including dimensions. The three datum reference planes are shown as A, B, and C. Headplates are manufactured from 1.6 mm (.063 inch) thick titanium 6Al-4V using common manufacturing methods.

b) Isometric view of headframe affixed to a mouse. Headplate shank projects posteriorly so as to not obstruct the mouse's field of view or impede on the mouse's ability to locomote.

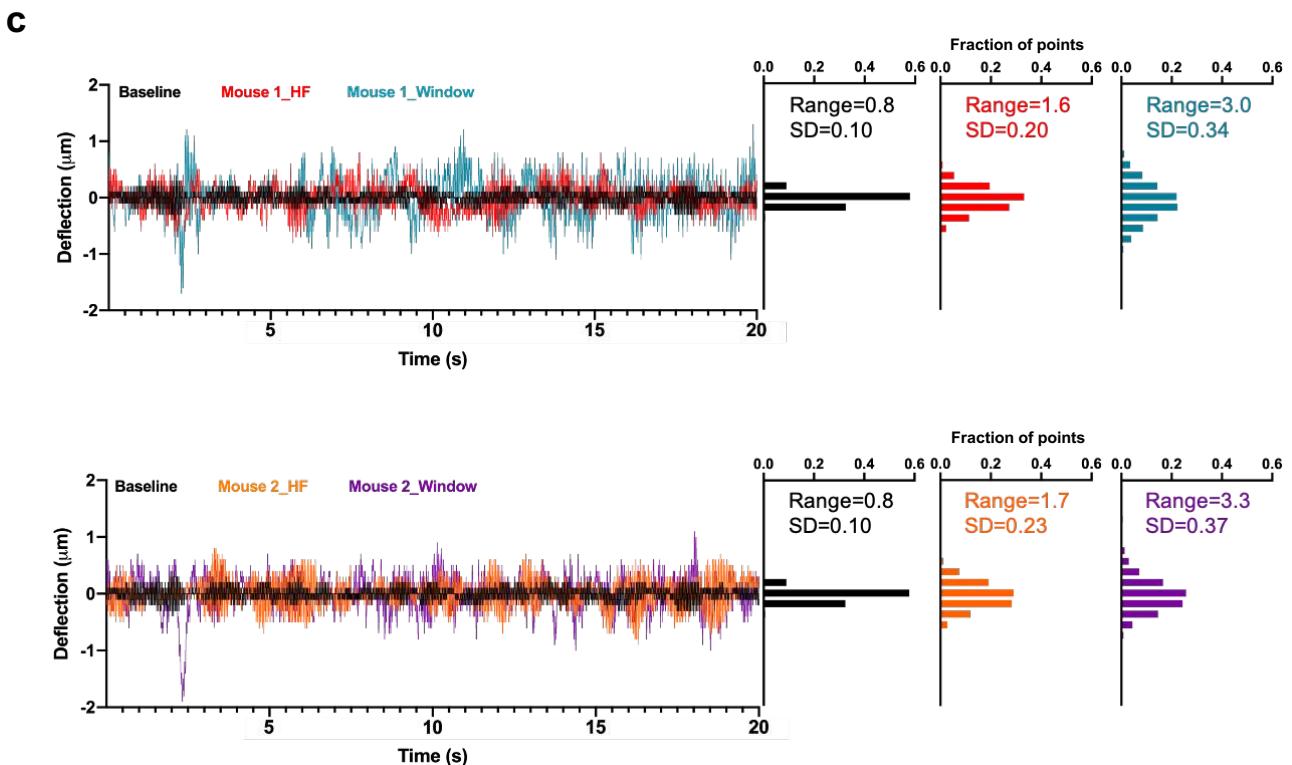
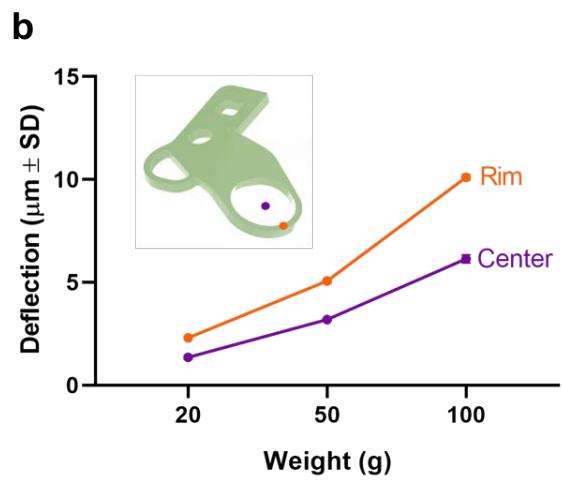
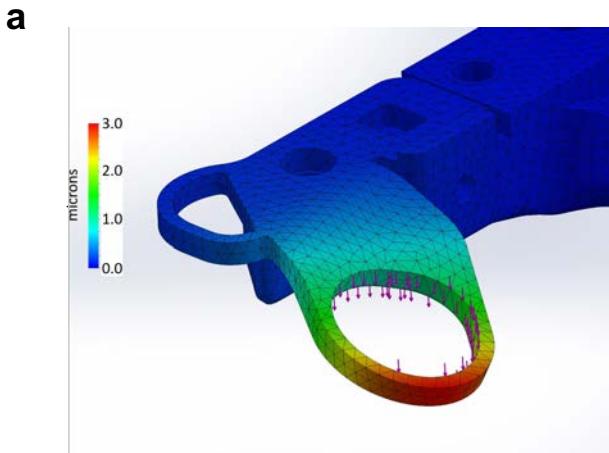


Figure 2. Headframe stiffness testing

a) Deflection simulations of the headplate and clamping mechanism suggested that a static .5N load applied to the headplate ring (shown as purple arrows) resulted in ~1.5-2 μm deflection at the center of the ring and a maximum of ~3 μm deflection at the outer edge of the ring.

b) Results of benchtop deflection tests indicated that a static load of 50g (~0.5N) applied to the rim of the headplate resulted in an average of 3.2 μm of displacement at the center of the headplate ring.

c) Deflection was next measured on the headframe (HF) and cranial window surface (Win) of two running mice that were head-fixed in an optical physiology instrument (Supplemental Figure 4a). Twenty-second samples of deflection data obtained from each point are shown, overlaid with the baseline noise measured on a headframe only (Baseline) clamped into the same system. As expected, deflection of the headframe during running increased over baseline and was greatest on the cranial window, as indicated by the increases in variance of the recorded signal (further shown as a broadening of the frequency distributions). However, the maximum deflection distances and ranges were well within our pre-determined tolerances.

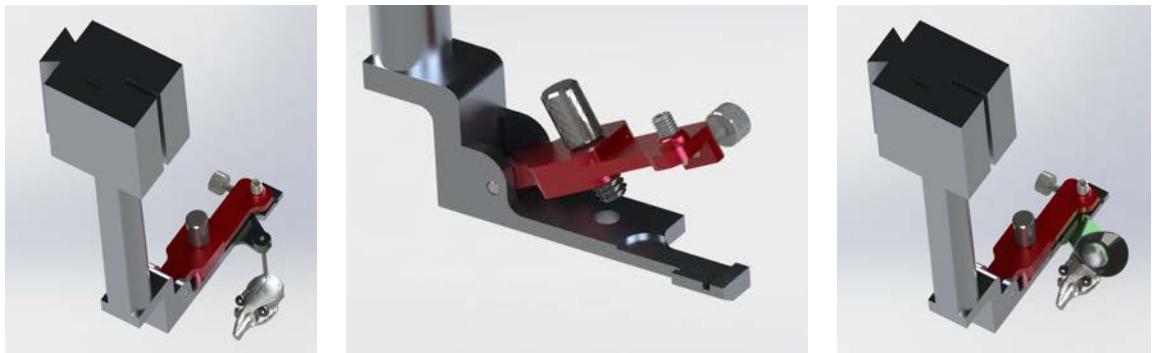
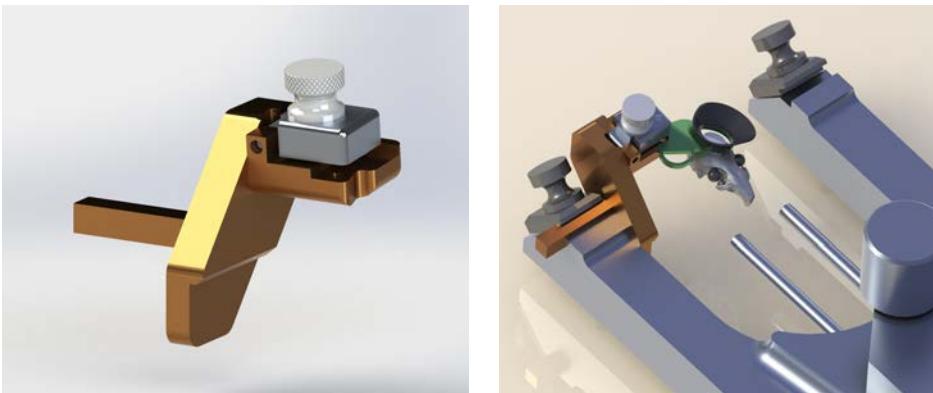
a**b****c**

Figure 3. Headframe surgical tooling.

a) LEFT: A “stylus” (blue), equipped with a shank identical to that of the headplate (green), is used to locate the mouse skull fiducial, lambda. RIGHT: This stylus places the headplate so that the center of the 10 mm headplate ring is located over the putative location of mouse visual cortex (M/L = -2.8mm, A/P = 1.3mm, with respect to lambda).

b) Custom headframe placement tool (“headframe clamp”) is compatible with the KOPF 1900 dovetail interface located on the Z-axis arm and places a clamshell-style clamp (CENTER) parallel to the levelled mouse skull. Once lambda is located with the stylus (LEFT) , it is replaced by the headframe (RIGHT) and lowered down along the Z axis to the skull for cementing.

c) The cranial window portion of the surgical procedure is facilitated by a custom “levelling clamp” (LEFT) that interfaces with the KOPF 1900 earbar clamp (RIGHT) and pitches the mouse forward 6 degrees. Once the entire earbar apparatus is rotated to 23 degrees, the cranial window plane is positioned perpendicular to gravity.

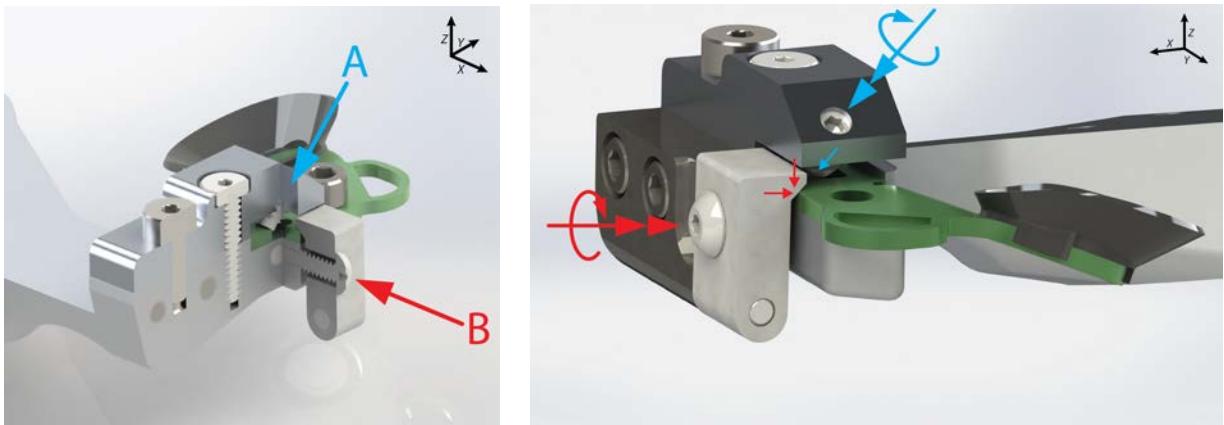
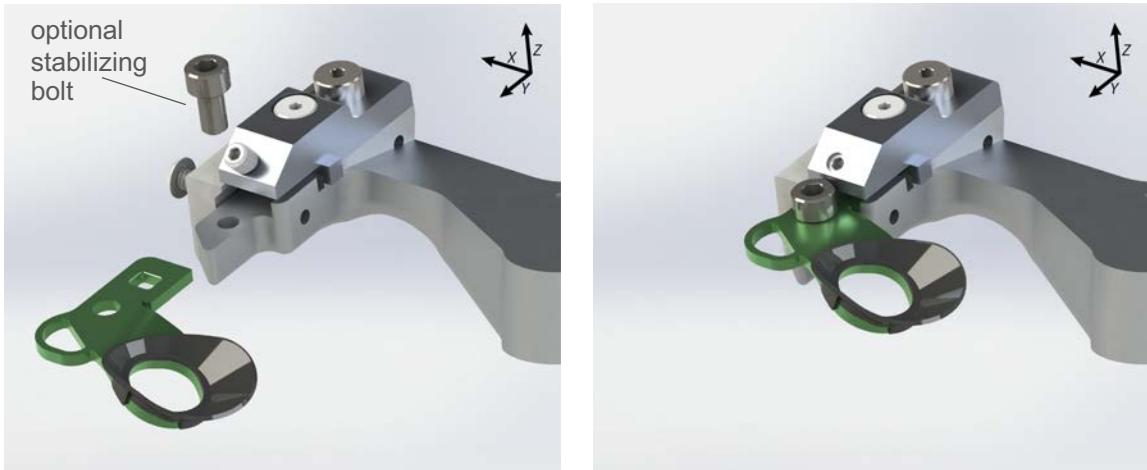
a**b**

Figure 4. Headframe clamping system.

a) Sectioned isometric view of the headframe clamping system exposes the two clamping bolts (A and B) that ensure proper seating of the headframe to the clamp. Two axial screw forces are applied to the headframe during installation. Red arrows show that axial screw force on the side bolt in the X direction resolves to both Z and X forces applied to the outer edge of the headframe shank and applies clamping pressure to datums A and C (Figure 2a). Blue arrows indicate that the axial screw force applied at 45 degrees in Z and Y resolves in the same forces and clamping pressures applied to the headframe in datums A and B.

b) The headframe is inserted into the clamp along the Y axis and once clamped, can be further secured using the optional socket head cap screw situated anterior to the front face of the clamp.

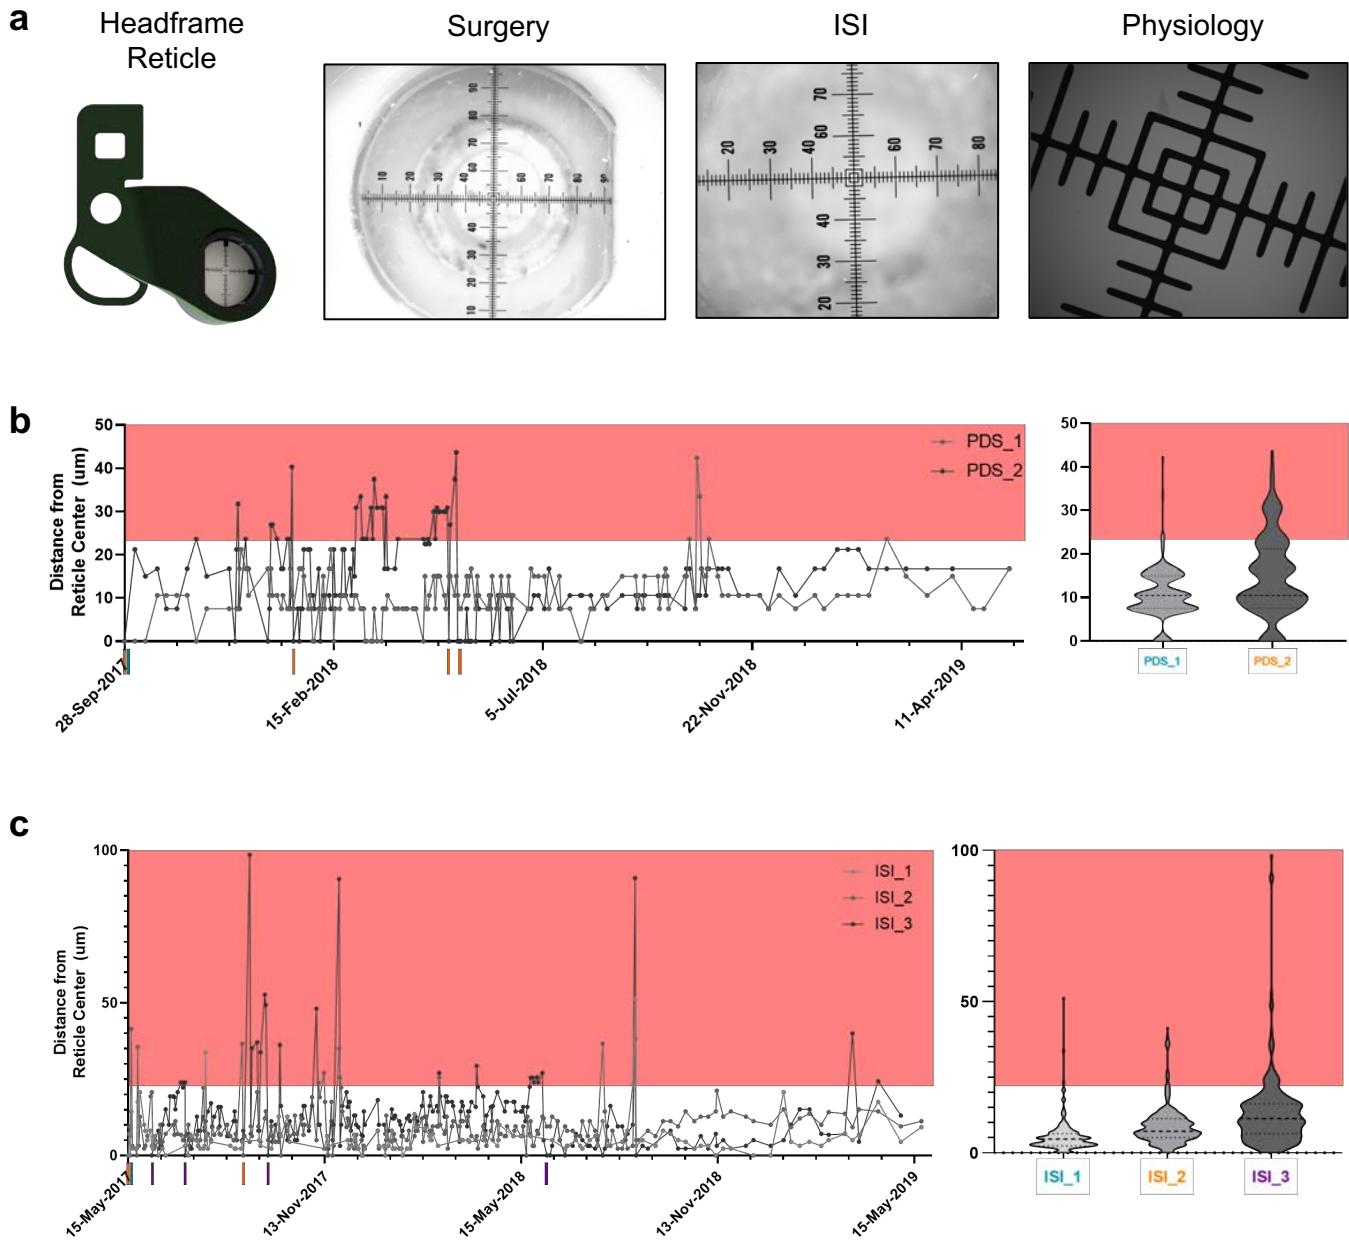


Figure 5. Pipeline system alignment and registration.

a) Systems were aligned to a set of headframe reticles. Example images from photodocumentation, intrinsic-signal imaging, and 2P microscopy instruments that were used for initial alignment and longitudinal monitoring. The images highlight the unique rotational, translational, and scaling attributes of each of the platforms.

b) Photodocumentation system registration monitoring data is shown for 2 instruments (PDS_1 & 2) over an 18-month period. Repeated detections of $>22.5\text{ }\mu\text{m}$ deviation from the registered reticile location triggered system re-registration (shown as colored hash marks). Median clamping variability over this time period was $10.61\text{ }\mu\text{m}$.

c) Intrinsic-signal imaging system registration monitoring data is shown for 3 instruments (ISI_1-3) over a 24-month period. Detections of $>22.5\text{ }\mu\text{m}$ of deviation from the registered reticile location triggered system re-registration (shown as colored hash marks). Median variability ranged from 4.5 to $11.25\text{ }\mu\text{m}$ depending on ISI instrument.

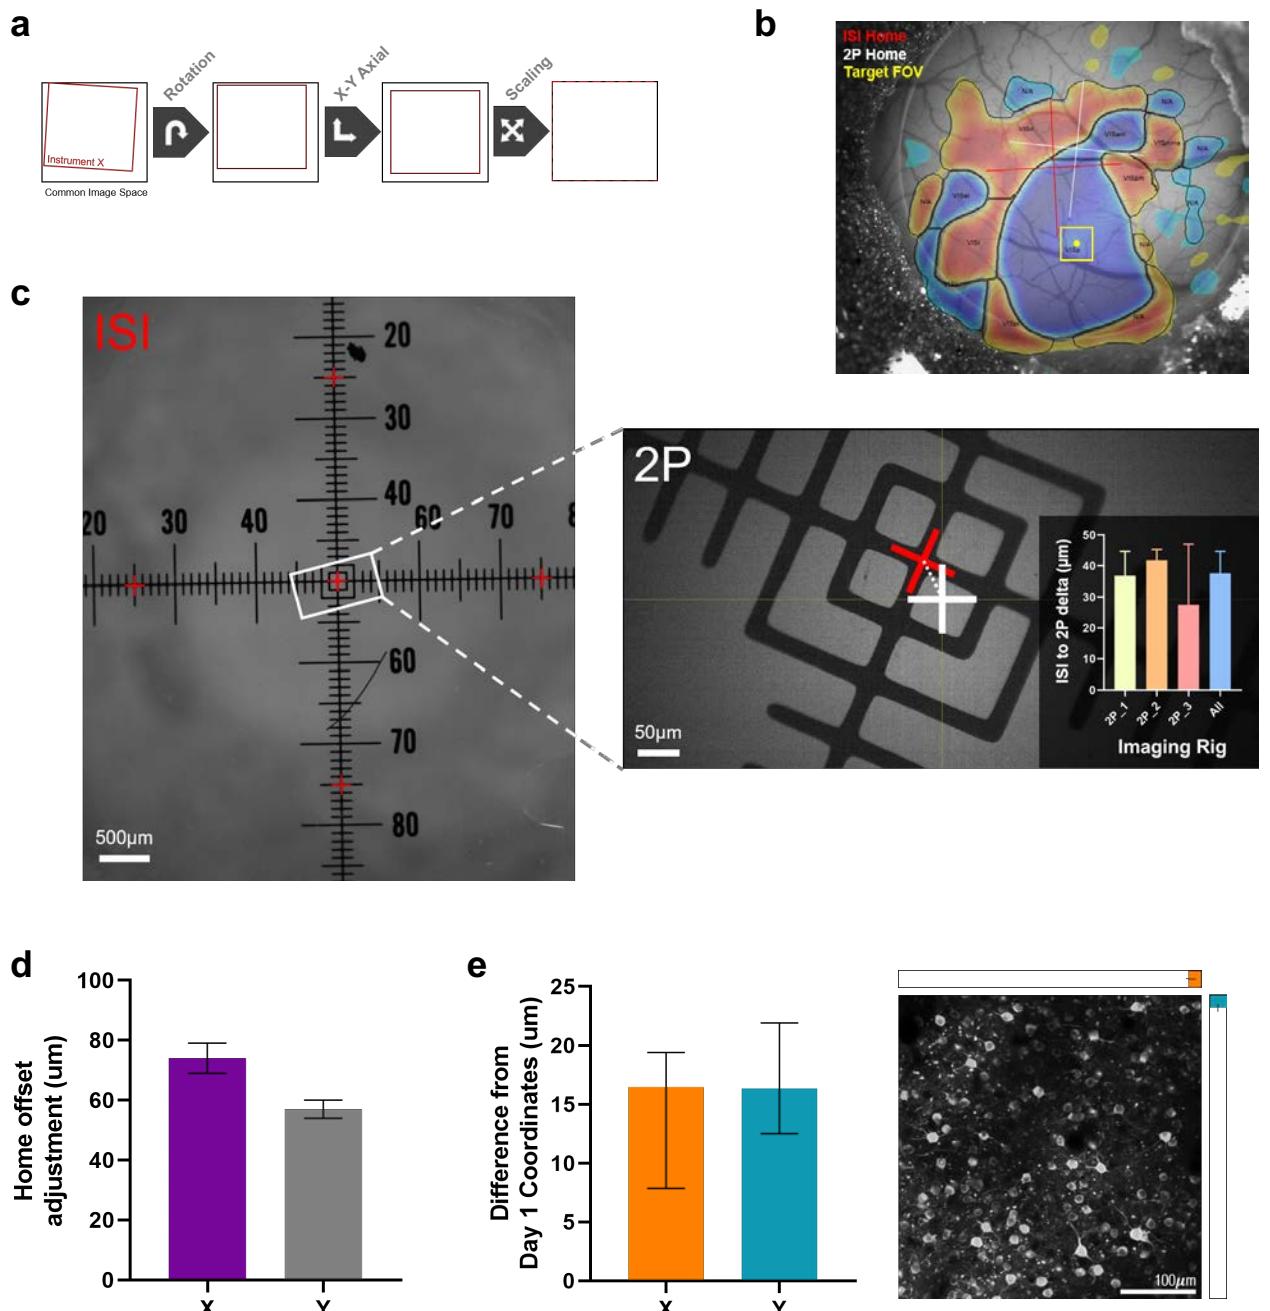


Figure 6. Cross-platform registration.



a) Cross-platform registration relied on transforming data collected with an individual pipeline instrument to a common reference space. These translations included rotation, X-Y axial, and scaling factors that were specifically calculated for each instrument during the reticle alignment process.

b) The *Allen Brain Observatory* leveraged cross-platform registration by using a set of ISI-defined coordinates to target 2P data collection of a retinotopically-defined region of cortex.

c) Reliability of ISI-2P registration is shown using a non-biological sample. Trial-to-trial variability of navigating to a set of 5 ISI-translated coordinates (red crosses) on multiple 2P microscopes. Across the three pipeline 2P rigs targeting was within 10-50 μm (median of “All”= 37.6 μm) of the desired location.




d) If necessary, before beginning an experiment operators were able to adjust the 2P home offset to adjust for biological motion and/or targeting inaccuracy. Median X and Y adjustments from a sample of >1700 experiments were 74 and 57 μm , respectively.

e) LEFT: Experimental data depicting the X and Y adjustments (median and 95% CI) that operators made to match a 2P field of view (FOV) across sessions. Operators made ~16um (median) of adjustment in both directions in order to match the FOV from the first session. RIGHT: An example 2P FOV (400x400 μ m), with the median X (orange) and Y (teal) adjustments shown to scale.

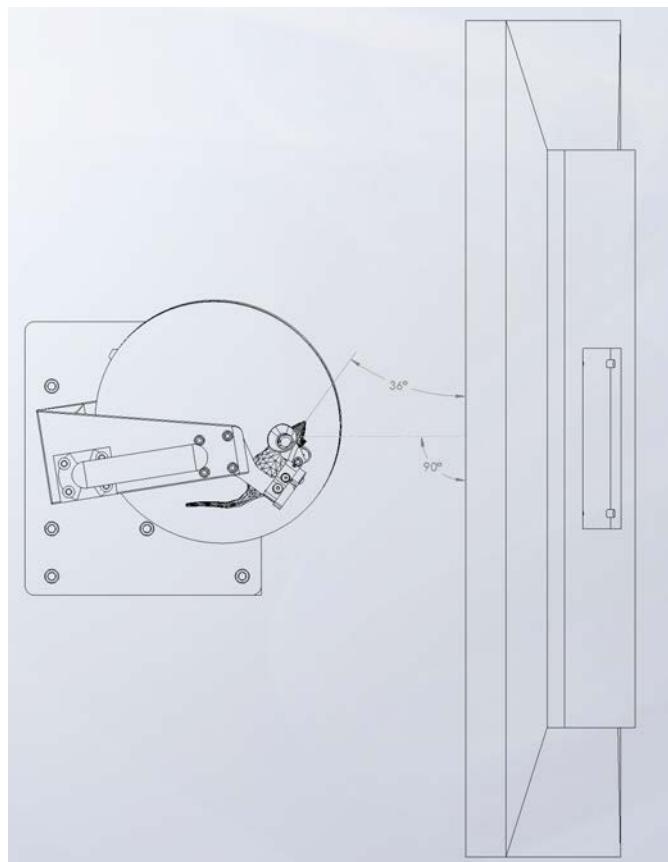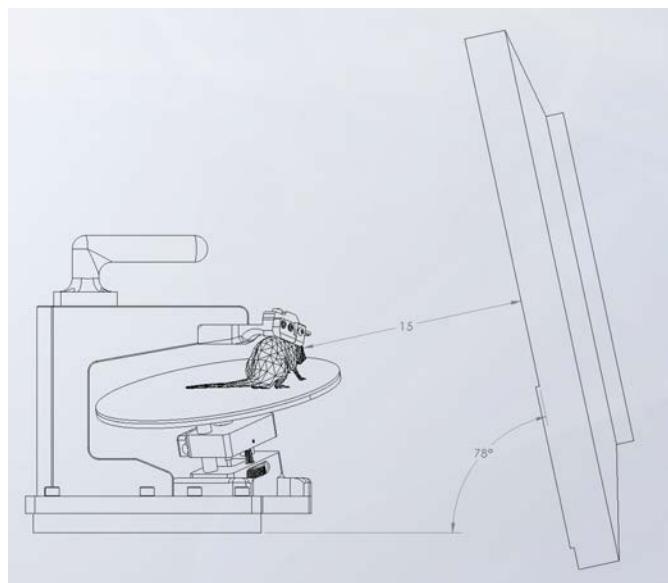a**b****Supplemental Figure 1. Brain Observatory pipeline mouse-to-screen geometry.**



a) Top-down view of the pipeline mouse-to-screen geometry. Mice are positioned at a 36° angle with respect to the screen.

b) Rear-view of the pipeline mouse-to-screen geometry. Mice are positioned 15cm from an LCD monitor, which is positioned at a 78° angle with respect to ground.

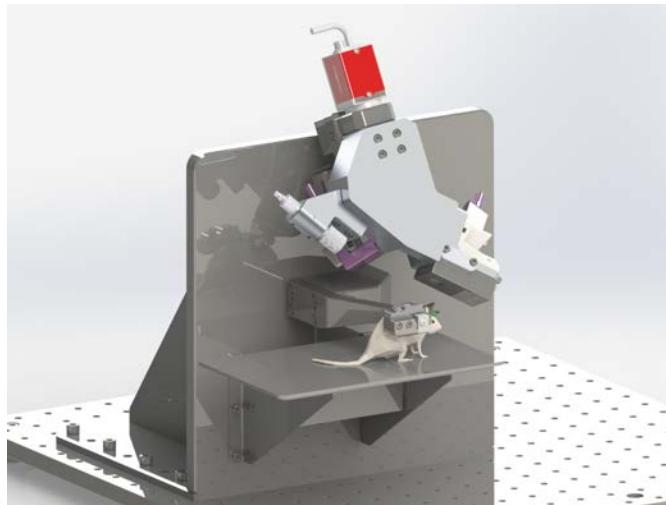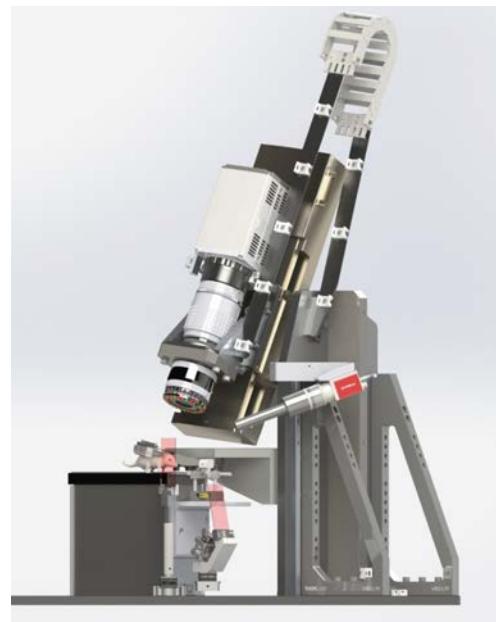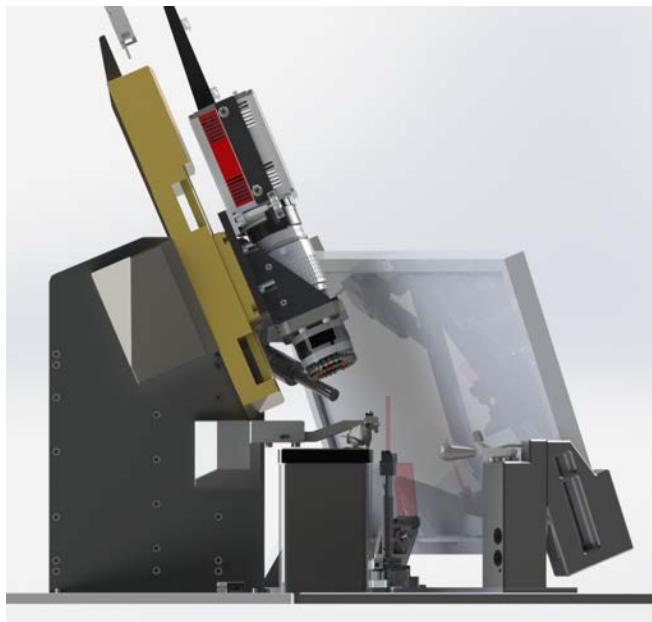a**b****Supplemental Figure 2. Surgical photo-documentation and Intrinsic-Signal Imaging pipeline systems.**

a) The surgical photo-documentation system was used to acquire registered images of the cranial window immediately following surgery. No visual stimulation was required.

b) The intrinsic-signal imaging systems (shown with and without the screen placed at a modified mouse-to-screen geometry) were used to acquire individualized maps of functional boundaries between visually-responsive regions of the mouse cortex. Systems included a camera (with ring-light LED illumination), eye-tracking camera (with LED illumination), and anesthesia machine (Somnosuite)

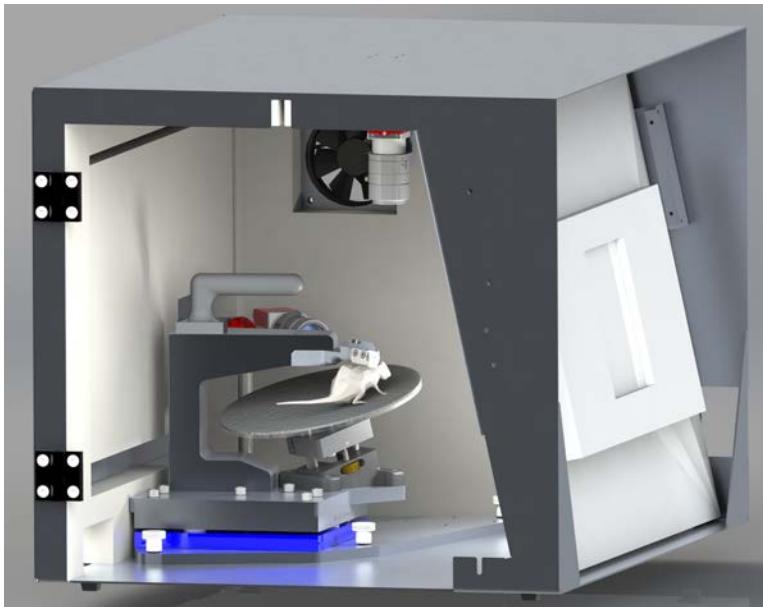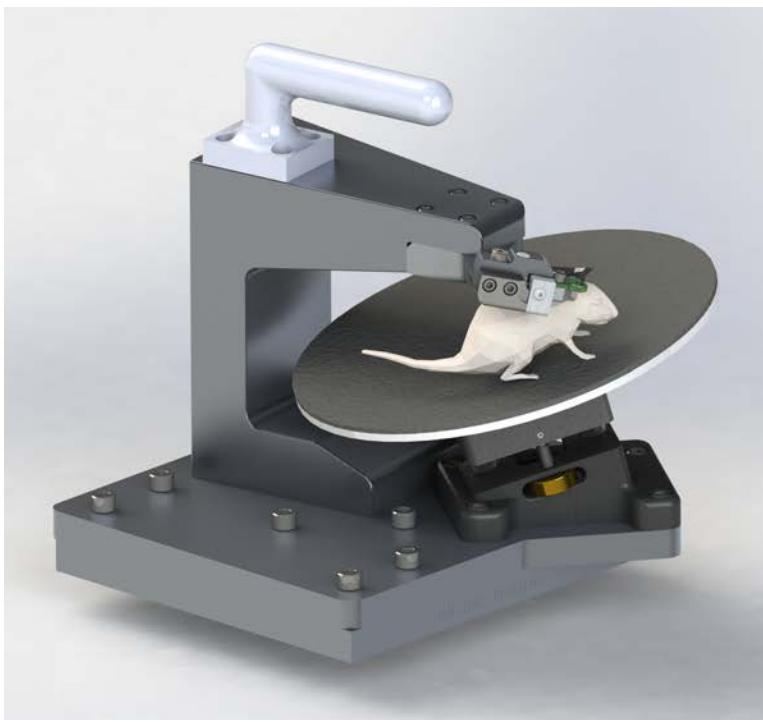a**b****Supplemental Figure 3. Behavioral enclosure and removable mouse head-fixation stage.**

a) Behavioral enclosures allowed for mice to be habituated to head-fixation and trained on visually-guided operant tasks. Front view of an enclosure (without door) shows a removable stage precisely positioned with respect to the stimulus screen using a kinematic mount (in blue). Enclosures are equipped with sound-attenuating foam, ventilation fan, body camera with illumination source, and a fluid delivery system mounted to a motorized 3-axis stage (not pictured).

b) The removable mouse stage allowed for mice to be head-fixed outside of the enclosure, an important factor in making the enclosures compact in size.

a

Brain Observatory_Scientifica


**b**

Brain Observatory_Nikon

**Supplemental Figure 4. Pipeline 2-photon microscopy platforms.**

a) Scientifica Vivoscope microscope (equipped with a 16X Nikon CFI LWD Plan Fluorite objective) with custom modifications to accommodate Brain Observatory mouse-to-screen geometry.

b) Nikon A1R MP+ microscope (equipped with a 16X Nikon CFI LWD Plan Fluorite objective) with custom modifications to accommodate pipeline mouse-to-screen geometry.

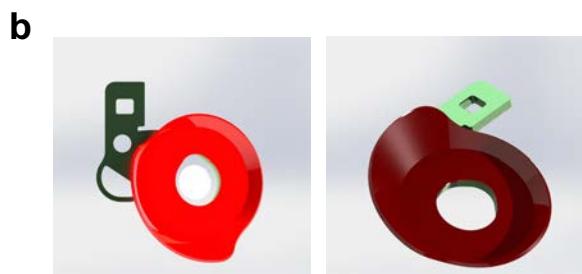

Supplemental Figure 5. Brain Observatory headframe variants.

- a) Headframe used for 2P imaging from lateral visual areas.
- b) Headframe and well used for 2P imaging with the Mesoscope microscope and objective.
- c) Headframe, well, and cap used for multi-probe electrophysiology recordings with Neuropixels probes.
- d) Headframe and well used for either through-skull, widefield imaging or stereotactically-guided probe insertion.
- e) Headframe used for electroencephalogram (EEG) arrays.